



**DETECTION OF IGE AGAINST MITE ALLERGENS  
USING TIME-RESOLVED FLUOROIMMUNOASSAY**

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์  
By  
**Ratchanoo Phiphatchaipaisarn**

**A Thesis Submitted in Partial Fulfillment of the Requirements for the Degree  
MASTER OF SCIENCE  
Department of Biology  
Graduate School  
SILPAKORN UNIVERSITY  
2010**

**DETECTION OF IGE AGAINST MITE ALLERGENS  
USING TIME-RESOLVED FLUOROIMMUNOASSAY**

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์  
By  
**Ratchanoo Phiphatchaipaisarn**

**A Thesis Submitted in Partial Fulfillment of the Requirements for the Degree  
MASTER OF SCIENCE  
Department of Biology  
Graduate School  
SILPAKORN UNIVERSITY  
2010**

การตรวจวัดระดับ IgE ต่อสารก่อภูมิแพ้ฝุ่นด้วย time resolved fluoroimmunoassay

โดย

นางสาวรัชฎา พิพัฒน์ชัยไพศาล

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

วิทยานิพนธ์นี้เป็นส่วนหนึ่งของการศึกษาตามหลักสูตรปริญญาวิทยาศาสตรมหาบัณฑิต

สาขาวิชาชีววิทยา

ภาควิชาชีววิทยา

บัณฑิตวิทยาลัย มหาวิทยาลัยศิลปากร

ปีการศึกษา 2553

ลิขสิทธิ์ของบัณฑิตวิทยาลัย มหาวิทยาลัยศิลปากร

The Graduate School, Silpakorn University has approved and accredited the Thesis title of “Detection of IgE Against Mite Allergens using Time-Resolved Fluoroimmunoassay” submitted by Miss Ratchanoo Phiphatchaipaisarn as a partial fulfillment of the requirements for the degree of Master of Science in Biology

.....  
(Assistant Professor Panjai Tantatsanawong, Ph.D.)  
Dean of Graduate School  
...../...../.....

The Thesis Advisor

1. Jundee Rabablert, Ph.D.
2. Assistant Professor Titiya Chittihunsa, Ph.D.
3. Assistant Professor Nat Malainual, Ph.D.

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

The Thesis Examination Committee

.....Chairman  
(Assoc. Prof. Renu Vejaratpimol, Ph.D.)  
...../...../.....

.....Committee  
(Assoc. Prof. Kornkarn Bramarapravati, Ph.D.)  
...../...../.....

.....Major-advisor  
(Jundee Rabablert, Ph.D.)  
...../...../.....

.....Co-advisor  
(Asst. Prof. Titiya Chittihunsa, Ph.D.)  
...../...../.....

.....Co-advisor  
(Asst. Prof. Nat Malainual, Ph.D.)  
...../...../.....

50303205: MAJOR : BIOLOGY

KEY WORDS : DER F 2/IGE/TIME-RESOLVED FLUOROIMMUNOASSAY

RATCHANOO PHIPHATCHAIPAISARN : DETECTION OF IGE AGAINST MITE ALLERGENS USING TIME-RESOLVED FLUOROIMMUNOASSAY. THESIS ADVISORS : JUNDEE RABABLERT, Ph.D., ASST. PROF. TITIYA CHITTIHUNSA, Ph.D., AND ASST. PROF. NAT MALAINUAL, Ph.D. 79 pp.

*Dermatophagoides farinae* and *D. pteronyssinus* are the prevalent house dust mites (HDM) in tropical countries and are associated with allergic diseases. This investigation developed a sandwich time-resolved fluoroimmunoassay (sandwichTRF) for the first time to detect specific IgE antibody in patients with skin prick test positive to HDM but no detectable IgE by other means. Levels of IgE to native and recombinant HDM allergens were measured by TRF in 50 HDM-allergic patients and 19 healthy subjects compared to sandwich enzyme-linked immunosorbent assay (sandwichELISA). A recombinant allergen, rDer f 2, showed a 14 kDa band corresponding to broad range proteins of native HDM. sandwichTRF employing of Df, rDer f 2 and Dp showed good correlations with sandwichELISA at  $r^2$  0.93-0.96. HDM IgE of Df, rDer f 2 and Dp detected from sandwichTRF are 62 %, 62 % and 50 % of allergic patient serum sample compared to 26 %, 32 % and 22 % detected from sandwichELISA, respectively. Sandwich TRF also detected 26.3 %, 31.6 % and 5.3 % positive samples from 19 healthy subjects while sandwichELISA showed 0 %, 5.3 % and 0 % IgE positive samples. The use of rDer f 2 as an HDM allergen for the assay was verified with no statistically different from other HDM allergens. Although with lower detection limit than sandwichELISA but sandwichTRF yielded higher sensitivity for patient sera with allergic symptoms but no detectable HDM IgE. It is indicated that TRF for HDM-specific IgE detection could play an important role in future diagnosis of HDM allergy.

---

Department of Biology Graduate School, Silpakorn University Academic Year 2010

Student's signature .....

Thesis Advisors' signature 1. .... 2. .... 3. ....

50303205 : สาขาวิชาชีววิทยา

คำสำคัญ : Der f 2/IgE/Time-Resolved Fluoroimmunoassay

รัชณู พิพัฒนชัยไพศาล : การตรวจวัดระดับ IgE ต่อสารก่อภูมิแพ้ไรฝุ่นด้วย time resolved fluoroimmunoassay. อาจารย์ที่ปรึกษาวิทยานิพนธ์ : อ. ดร. จันทร์ดี ระแบบเลิศ, ผศ. ดร. ทติยา จิตติहरรรยา และ ผศ. ดร. ฌัฐ มาลัยนวน. 79 หน้า.

ไรฝุ่น *Dermatophagoides farinae* และ *D. pteronyssinus* เป็นไรฝุ่นบ้านที่พบเห็นได้บ่อยๆ ในประเทศเขตร้อนชื้น และเป็นสาเหตุสำคัญของการก่อให้เกิดโรคภูมิแพ้ ในการศึกษานี้เป็นการพัฒนาวิธี sandwich time-resolved fluoroimmunoassay (sandwichTRF) เพื่อตรวจวัดแอนติบอดี IgE ในผู้ป่วยที่ให้ผลบวกด้วยวิธี skin prick test แต่ไม่สามารถตรวจวัดได้ด้วยวิธีอื่น ๆ โดยใช้ซีรัมจากผู้ป่วยโรคภูมิแพ้ 50 คน และจากผู้ที่สุขภาพแข็งแรง 19 คน แล้วเปรียบเทียบกับผลการตรวจด้วยวิธี sandwich enzyme-linked immunosorbent assay (sandwichELISA) ผลการศึกษายืนยันว่า โปรตีนสังเคราะห์ rDer f 2 มีขนาดโปรตีน 14 kDa เท่ากับโปรตีนสารก่อภูมิแพ้ในธรรมชาติ ระดับแอนติบอดี IgE ที่วัดด้วยวิธี sandwichTRF ต่อโปรตีนสารก่อภูมิแพ้ของไรฝุ่น Df, rDer f 2 และ Dp มีความสัมพันธ์กับวิธี sandwichELISA ( $r^2$  0.93-0.96) จากการเปรียบเทียบพบว่า วิธี sandwichTRF สามารถหาค่าแอนติบอดี IgE ต่อ Df, rDer f 2 และ Dp ได้ที่ระดับ 62, 62 และ 50 เปอร์เซ็นต์ของผู้ป่วยโรคภูมิแพ้ ส่วนวิธี sandwichELISA วัดได้เพียง 28, 32 และ 22 เปอร์เซ็นต์ตามลำดับ สำหรับผู้ที่มีสุขภาพแข็งแรง 19 คน วิธี sandwichTRF สามารถตรวจหาค่าแอนติบอดี IgE ต่อ Df, rDer f 2 และ Dp ได้ที่ระดับ 26.3, 31.6 และ 5.3 เปอร์เซ็นต์ ส่วนวิธี sandwichELISA วัดได้ 0, 5.3 และ 0 เปอร์เซ็นต์ตามลำดับ ผลการใช้ rDer f 2 และสารก่อภูมิแพ้ไรฝุ่นในการศึกษานี้ผลการตรวจแอนติบอดี IgE ด้วยวิธี sandwichELISA และ sandwichTRF ไม่แตกต่างกันทางสถิติ แต่พบว่าวิธี sandwichTRF สามารถตรวจพบแอนติบอดี IgE ได้ในระดับที่ต่ำและให้ผลที่ดีกว่าวิธี sandwichELISA ในผู้ป่วยโรคภูมิแพ้ จากผลการศึกษาสรุปได้ว่าวิธีตรวจวัดระดับแอนติบอดี IgE ด้วยวิธี sandwichTRF เป็นวิธีการทางห้องปฏิบัติการวิธีหนึ่งที่เหมาะสมในการวินิจฉัยผู้ป่วยโรคภูมิแพ้

ภาควิชาชีววิทยา

บัณฑิตวิทยาลัย มหาวิทยาลัยศิลปากร

ปีการศึกษา 2553

ลายมือชื่อนักศึกษา .....

ลายมือชื่ออาจารย์ที่ปรึกษาวิทยานิพนธ์ 1. .... 2. .... 3. ....

## ACKNOWLEDGEMENT

I wish to express my sincere gratitude and deep appreciation to Dr. Jundee Rabablert, my advisor, for her guidance, invaluable advice, supervision and encouragement throughout this study. I am also grateful to Assistant Professor Dr. Nat Malainual, Department of Parasitology, Faculty of Medicine Siriraj Hospital, Mahidol University for his suggestion and guidance. I would like to thank Assistant Professor Dr. Surapon Piboonpocanun, Institute of Molecular Biosciences, Mahidol University for providing native and recombinant house dust mites.

My appreciation is also expressed to Associate Professor Dr. Kornkarn Bramarapravati, Department of Preclinical Science, Faculty of Medicine, Thammasat University for reviews and recommendations and Dr. Naowarut Meejung, Department of Statistic, Faculty of Science, Silpakorn University and Assistant Professor Dr. Junya Pattaraarchachai, Department of Preclinical Science, Faculty of Medicine, Thammasat University for statistics on this thesis. I would like to express to Associate Professor Dr. Renu Vejaratpimol, Assistant Professor, Dr. Titiya Chittihunsa for recommendation on my thesis. This study was supported by Thailand Research Fund No. MRG-WII505S061, partial fund from Thailand Research Fund No. MRG-WII525S092 and Thailand Research Fund No. DIG5180004.

Special thanks are also expressed to Dr. Nares Wongpitoon and Dr. Worawan Durongpisitkul, Department of Pediatric, Police General Hospital for kindly providing blood samples of allergic Thai donors. My special thank for their kindness in providing blood samples of patients and the donors from Silpakorn University, Nakorn Pathom, Thailand. My appreciation is also extended to Mr. Duangthep Thongdee and Miss Sasipa Thanyaratsrisakul for their friendship and support. I am also indebted to all my friends, staff members of Department of Parasitology, Faculty of Medicine Siriraj Hospital for their friendships, generosity and sharing the happy time throughout my studying.

Finally, I am grateful to my beloved parents and family for their love, kindness support, encouragement and understanding throughout my study.

Ratchanoo Phiphatchaipaisarn

## TABLE OF CONTENTS

	Page
English Abstract.....	d
Thai Abstract.....	e
Acknowledgment .....	f
List of Tables .....	j
List of Figures .....	k
Chapter	
1. Introduction.....	1
2. Literature review .....	3
Allergic disease .....	3
IgE mediated reactions .....	4
Anaphylactic reactions .....	7
House dust mite allergens .....	8
Immunity against House-dust mite allergen .....	12
Antibody response.....	12
T-cell response .....	13
Laboratory diagnosis of allergic diseases.....	15
<i>In vivo</i> .....	15
<i>In vitro</i> .....	16
3. Materials and methods .....	20
House dust mite (HDM) allergens .....	20
Preparation of House dust mite allergen .....	20
Determination of HDM protein.....	21
Characterization of HDM allergen.....	21
Subjects .....	22
Immunological analysis.....	23
Enzyme-linked immuosorbent assay (ELISA).....	23
Evaluation of coating concentration of allergens.....	23
Evaluation of subject's serum .....	23



Chapter	Page
Evaluation of biotinylated-labeled mouse anti-human IgE antibody .....	24
Time resolved fluoroimmunoassay (TRF) .....	24
Sandwich enzyme-linked immuosorbent assay (sandwichELISA).....	24
Sandwich time resolved fluoroimmunoassay (sandwichTRF).....	25
Statistic analysis .....	26
4. Results.....	27
HDM–allergen characteristics.....	27
Subject characteristics .....	28
The optimization of ELISA condition for specific IgE detection .	32
The optimization of allergen concentration .....	32
The optimization of serum dilution.....	32
The optimization of biotinylated-labeled mouse anti-human IgE antibody .....	32
Calibration curve of specific IgE detected with all HDM allergens	34
Calibration curve between OD unit and $kU_A/l$ using sandwichELISA .....	34
Calibration curve between counts per second and $kU_A/l$ using sandwichTRF.....	35
Measurement of specific IgE to HDM allergens.....	38
Specific IgE to HDM allergens using sandwichELISA .....	38
Specific IgE to HDM allergens using sandwichTRF .....	38
5. Discussion .....	47
6. Conclusion .....	50
Reference .....	51
Appendix.....	66
Appendix A.....	67

	Page
Appendix B .....	70
Appendix C .....	76
Biography.....	79

# มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

## LIST OF TABLES

Tables		Page
1	Molecular cloning of <i>Dermatophagoides</i> spp. allergens .....	9
2	List of commercial allergens used for select the patient groups. ....	28
3	Demographic and characteristics of the study individuals. ....	29
4	Profiles of 69 subjects responded to panel of allergens sensitization. ....	30
5	Optimization of Df, rDer f 2 anf pPICZ concentrations for the detection of specific IgE. Various allergens concentrations (250, 500 and 1000 ng/ml) were evaluuated in the experiments. The serum and biotinylated-labeled mouse anti-human IgE antibody diluted 1:10 and 1:1000, respectively by ELISA.....	33
6	Optimization of Df, rDer f 2, Dp and pPICZ concentrations for the detection of specific IgE. Allergens concentrations 1000 ng/ml was evaluuated in the experiments. The biotinylated-labeled mouse anti-human IgE antibody diluted 1:1000. The serum diluted 1:2 and 1:10, respectively by ELISA.....	33
7	Optimization of Df, rDer f 2 and pPICZ concentrations for the detection of specific IgE. Allergens concentrations 1000 ng/ml was evaluuated in the experiments. The serum diluted 1:10. The biotinylated-labeled mouse anti-human IgE antibody diluted 1:1000 and 1:2000, respectively by ELISA.....	34
8	Profiles of 50 allergic patients detected specific IgE to Df, rDer f 2, Dp and pPICZ. ....	40
9	Profiles of 19 Healthy subjects detected specific IgE to Df, rDer f 2, Dp and pPICZ. ....	43
10	Number of positive samples from sandwichELISA and sandwich TRF in allergic patient and healthy participant serum as seen using Df, rDer f 2 and Dp allergen against group II mAb.....	44
11	SandwichTRF positive cases in serum from allergic patients categorized by sandwich ELISA result in Df, rDer f 2 and Dp testing.....	44

## LIST OF FIGURES

Figures		Page
1	The protein components of HDM allergen were determined by SDS-PAGE a); Lane 1:Df; Lane 2: Dp; Lane 3: Molecular mass standards (in kDa); Lane 4: rDer f 2; Lane 5: pPICZ. b) Western blot Lane 3: Molecular mass standards (in kDa); Lane 4: rDer f 2; Lane 5: pPICZ .....	27
2	Calibration curve for sandwichELISA for a) Df, b) rDer f 2 and c) Dp... ..	36
3	Calibration curve for sandwichTRF for a) Df, b) rDer f 2 and c) Dp... ..	37
4	Correlation between levels of specific IgE against a) Df, b) rDer f 2 and c) Dp measured by sandwichELISA and sandwich TRF.....	45
5	SandwichTRF positive cases from serum of allergic patients tested with all three HDM allergens. Median, standard deviation, 25 and 75 percent values are presented. ....	46

## CHAPTER I

### INTRODUCTION

House-dust mites (HDM) represent one of the most important allergen sources for the development of allergic diseases worldwide, particularly asthma and allergic rhinitis. *Dermatophagoides farinae* (Df, originally known as American HDM) and *Dermatophagoides pteronyssinus* (Dp, European HDM) are the predominant species in tropical and subtropical climates. More than 80% of allergic patients have been found to be sensitive to house dust mite allergens worldwide (73, 79). Positive skin prick tests (SPT) or serum Immunoglobulin (Ig) E antibodies to HDMs were demonstrable in allergic patients. However, if patients were allergic to histamine, SPT could lead to complicated immunoreaction harmful to the patients (122). Enzyme-linked immunosorbent assay (ELISA) was the method used to quantify serum HDM-IgE *in vitro* in laboratories (14). However, a more sensitive *in vitro* test is needed for people who had dust mite allergic clinical diagnosis but shown undetectable HDM-IgE in their sera. Monoclonal antibodies (mAbs) had been frequently used in allergy research. Their uses included the quantification of environmental allergen (18), allergens purification (35) and crystal structure (105). Specificity for unique epitopes and unlimited *in vitro* production capability are the advantage of allergen-specific mAbs.

Time-resolved fluorescent resonance energy transfer (TRF) was developed to measure Plasma vascular endothelial growth factor concentrate in 92 healthy controls, in 36 benign stomach disease patients and in 92 gastric cancer patients before surgery. (90). TRF was evaluated with a panel of serum samples from infected (n = 73) and uninfected (n = 480) sources of Brucellosis and compared to the performance of the parent cELISA, an indirect ELISA (iELISA) and fluorescence polarization assay (FPA). The performance of the TR-FRET assay matched the performance of the iELISA, which had 100% diagnostic sensitivity and specificity, and surpassed the performance of the cELISA and the FPA. The results also demonstrated that the TR-FRET technique was effective with poor-quality serum samples from the field (66).

The purpose of our study was to evaluate a rapid and convenient fluorometric method based on time resolved fluorescence of on  $\text{Eu}^{3+}$  chelate to analyze HDM-specific IgE and to compare it with the established ELISA method. We evaluated HDM-specific IgE levels in allergic patients and healthy subjects.

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

## CHAPTER II

### LITERATURE REVIEW

#### 1. Allergic disease

Allergic diseases were produced by immunological hypersensitivity reactions to otherwise harmless substances caused by proteins called allergens. These reactions were included in the term “allergy”. The word allergy was introduced by Von Pirquet in 1906 to designate “altered reactivity” as a result of previous exposure. Allergy was mostly used as general term for reaction of discomfort of unknown origin (86). The most common allergic diseases were associated with type 1 hypersensitivity where the allergen induced IgE antibody production and sensitized T cells to produce TH2 cytokines. The effects produced by atopic or anaphylactic reaction were the results of teophase system. The sensitization phase was initiated by antigen presenting cells uptake antigen and presents the digested fragment to naïve T cells, which led to the T-cell proliferation, differentiation, cytokine production and the subsequently induced high specific IgE production from B cells. The other phase, elicitation phase, occurs upon by re-exposure to the same allergen. Following reaction, at least 2 molecules of specific IgE which bounded to the FcεRI on the mast cells and basophils were crosslinked with allergens leads to the release biological substances including histamine, heparin and serotonin. These mediators were transformed by other immunological cells into prostaglandin and leukotrienes which were responsible for the late phase allergic reaction. The effect of these mediators included smooth muscle contraction, increased vascular permeability, gastric nasal and lacrimal secretion. The type of reaction depends upon the dose of allergen, the route of contact allergen, the frequency of contact with allergen and the degree of sensitivity of involved individual. Allergic diseases were multifactorial diseases. Factors that were found to influence the occurrence of allergies were the host and environment. Host factors involved in the risk for allergy were heredity, sex, race and age, with heredity being by far the most important. Persons who had a family history of allergic diseases would be at a high risk of developing the diseases. Environmental factors could act as the trigger in agent such

as allergens, or acted like an adjuvant such as passive smoking and pollution (9). In general, an exposure dose was determined by two factors: the exposure concentration and the exposure time. For allergens, the exposure concentration was uncertain. For house dust mite, allergen particles contaminated infested fabrics and then became airborne with disturbance. Particles were cleared by settling, but some were also absorbed onto walls, furniture, and other reservoirs. Most studies of exposure had measured allergen levels in settled dust; only rarely airborne concentrations had been assessed. Settled dust and airborne dust mite allergen concentrations were highly variable, with reported coefficients of variation of 30% or more (132).

It has been reported that two reactions played a role in allergic diseases such as IgE-mediated reactions and anaphylactic reactions

### 1.1 IgE-mediated reactions

*D. farinae* and *D. pteronyssinus* were identified in house dust samples from all over the world since 1964 (121). An evidence of exposure to the HDM allergens *D. farinae* and *D. pteronyssinus* was an important risk factor for allergic sensitisation, asthma development and asthma symptom exacerbation (101). Studies of house dust-allergic individuals around the world had shown that house dust mites caused symptoms such as perennial-type asthma, rhinitis and conjunctivitis, often with nocturnal or early morning episodes (65). In Thailand, allergic conditions have been very common among children residing in Bangkok (57, 80). Teeratakulpisarn J, et al (2000) showed the four-fold rising of allergic diseases during the last decade. Number of incidences revealed that about 13% or 2,000,000 of paediatric population were suffering from allergic diseases and a large number of them were reported by the symptoms of asthma and rhinitis (118). House dust was heavily contaminated, but removal was difficult because of the inaccessible reservoirs (77).

The other constituents of native *D. pteronyssinus* allergens, but not Der p 1 or Der p 2, did not significantly influence on the IgE-mediated early asthmatic responses but contributed significantly to the allergen-induced late asthmatic response and bronchial hyperreactivity (117). *D. pteronyssinus* had also been reported to play an important role as a trigger in patients with atopic dermatitis, including adult patients (60). However, in a cross-sectional study of 1669 school beginners 6 to 7 years old in Augsburg (Bavaria, Germany), it was concluded that current eczema in these children



were related to Der f 1 exposure and not to Der p 1 exposure (59). Patients who had been induced by house dust mite allergen for more than 48 hours continuously and contributed to eczematous eruptions were characterised by considerably increased levels of IgE antibodies, high activity of atopic dermatitis (50). It was possible that a number of features described to *D. pteronyssinus* would be applicable to *D. farinae* but had not specifically been investigated for this mite. The reader was referred to the entry on *D. pteronyssinus*. Various studies reported that the rate of sensitisation was higher among atopic children and that high mite infestation increased the rate of sensitisation. The European Community Respiratory Health Survey, an international study of asthma prevalence and risk factors for asthma, collected information on IgE antibodies to common allergens in over 13,000 adults living in 37 centres in 16 countries and found a median prevalence of 20.3% (range 6.7-35.1%) for sensitisation to *D. pteronyssinus* (13). In a follow up study, home visits with 3580 participants from 22 study centres in the European Community Respiratory Health Survey II were conducted; mattress dust was sampled and analysed for Der p 1 and Der f 1, which allergens were detectable ( $\geq 0.1$  mg/g) in 68 and 53% of the samples, respectively. Large differences in allergen levels among study centres were observed, and geographic patterns for Der p 1 and Der f 1 were different. Low winter temperatures reduced Der p 1 but not Der f 1 (133). *D. farinae* and *D. pteronyssinus* appear to be significant allergens in most geographic regions but may vary within these regions. In a study in the homes of 111 asthmatic children in 3 climatic regions in Sweden, the major allergen Der m 1, together with Der p 1 from *D. pteronyssinus* and Der f 1 from *D. farinae* was analysed. Der f 1 was the predominant house dust mite allergen, Der p 1 was the least often found, and Der m 1 represented 31% of the allergen load. However, in the Linköping area Der m 1 was the major house dust mite allergen (58%). Of the children with IgE antibodies against house dust mite, 67% reacted to all 3 mites. Mite sensitisation rates were marginally increased (7%) by the addition of IgE analysis of *D. microceras* to the routine analysis of IgE antibodies against *D. pteronyssinus* and *D. farinae*. The authors concluded that Der m 1 may in this instance be an important house dust mite allergen and should be considered when House dust mite exposure data were assessed in areas with a climate like that of Sweden (119). However, in another Scandinavian population, in Denmark, a study found that both immunochemically and microscopically, *D. farinae* was

dominant, *D. pteronyssinus* less frequent but important, and *D. microceras* insignificant (93). In a study assessing specific allergen content in dust samples from the homes of 106 allergy clinic patients in Baltimore in the USA, House dust mite allergens were detected in 99% of homes. *D. farinae* was found in 95%, *D. pteronyssinus* in 88% and *D. microceras* in 31%. Although sensitisation to these allergens was not evaluated, the study indicates that *D. microceras* may be an important allergen in this geographical region (123). In tropical Singapore, a prospective evaluation was made of 175 newly diagnosed allergic rhinitis patients, of whom 39% reported a concomitant diagnosis and/or clinical complaints of bronchial asthma and 48% of atopic dermatitis; skin reactivity for *D. pteronyssinus* and *D. farinae* mix was detected in 85% of patients (and 62% for *B. tropicalis*) (56). In studies of house dust in Bursa, Turkey, approximately 34% of houses were found to be infested with House dust mites. The rate of infestation was 18.75% and 50% in the houses with and without central heating systems, respectively. The prevalence of *D. pteronyssinus* was found to be 58.34%, compared with 16.67% for *Glycophagus domesticus* and 4.16% for *D. farinae* (41). In an evaluation of house dust collected from dwellings at 7 locations in Upper Silesia, Poland, mites were found in 56.1% of the samples. *D. farinae* was predominant (75.3%), followed by *D. pteronyssinus* (18.6%) and *Euroglyphus maynei* (1.5%) (99). A number of studies in South America had documented the significance of *D. pteronyssinus* sensitisation. In Valdivia, Chile, out of 100 consecutive paediatric asthma patients evaluated, 80 were confirmed to have skin reactivity to at least 1 mite species. All patients with skin reactivity for mites were positive to *D. pteronyssinus*, and 99% to *D. farinae*. All of the patients with severe persistent asthma had skin reactivity to mites, as did 85% in the moderate group, and 73% in the mild group. Ninety-five percent of patients with asthma and allergic rhinitis were shown to have skin reactivity to mites, as were 92% of patients with asthma and eczema and 100% of patients with asthma, allergic rhinitis and eczema (15). In a study of patients with allergic respiratory disease attending an allergy clinic in Brazil, out of 212 medical records evaluated, 61.7% showed sensitisation to Der p, 59.9% to Der f and 54.7% to Blo t (97). In a study of 579 asthmatic patients in Taiwan, it was shown through measuring allergen-specific IgE antibodies that almost 59% were sensitised to *D. microceras*, compared to 59.8% to *D. pteronyssinus* and 56.8% to *D. farinae*.

Sensitisation to Cockroach was found in 38.3%, to Dog dander in 26.3%, to *Candida albicans* in 13.3%, to Cat dander in 10% and to *Cladosporium herbarum* in 6.6%. The study indicates the importance of considering *D. microceras* when evaluating allergic individuals (22). Among 93 Taiwanese asthmatic children aged 3 to 15 years evaluated for sensitisation to 5 species of mites, 63 were found to have IgE antibodies to at least 1 of the following mites: *D. pteronyssinus*, *D. farinae*, *D. microceras*, *Euroglyphus maynei*, and *Blomia tropicalis*. Sensitisation to *D. pteronyssinus* was found in 87%, to *D. farinae* in 85%, to *D. microceras* in 84%, to *Euroglyphus maynei* in 77% and to *Blomia tropicalis* in 65% (61). Similarly, in a Taiwanese study of 498 atopic children aged 2 to 16 years, high prevalences of sensitisation were documented: 90.2% to *D. pteronyssinus*, 88.2% to *D. farinae*, 79.5% to *D. microceras*, and 76.7% to *Blomia tropicalis* (46).

A group of 25 atopic children under 11 years of age in Oxford in the United Kingdom was studied for skin reactivity and IgE antibodies to 4 species of House dust mites: *D. pteronyssinus*, *D. farinae*, *D. microceras* and *Euroglyphus maynei*. All of the children were sensitised to *D. pteronyssinus* and 80% of these children were also sensitised to *D. farinae* and *D. microceras*. Importantly, dust samples from various sites in the homes of the children revealed *D. pteronyssinus* in all the homes, but no *D. farinae* or *D. microceras*. A control group of 20 atopic children of similar ages who were not sensitised to HDM allergens had similar exposure to the 4 mite species. These results suggest that factors in addition to mite exposure were important in the development of specific IgE responses to house dust mites (130). Interestingly, in habitats where conditions were not favourable for mites, mites had still managed to survive and may cause sensitisation. The presence of *D. farinae* and *D. pteronyssinus* had been reported in Egypt (27). A large body of studies from around the world had demonstrated the relevance of this allergen (112). The reader was referred to references listed in the first paragraph of this section for more detailed clinical information.

### **1.2 Anaphylactic reactions**

Systemic anaphylaxis could occur after the ingestion of heated or unheated mitecontaminated foods. This problem may be more prevalent in tropical and subtropical countries than previously recognised. The most common symptoms

following the ingestion of mite-contaminated flour were breathlessness, angioedema, wheezing, and rhinorrhea, and these started between 10 and 240 minutes (min) after eating (82).

## **2. Housedust mite allergens**

As shown in Table 1, HDM allergens were grouped based on their biological function. According to the International Union of Immunological Societies (IUIS) Allergen Nomenclature Subcommittee, the designation for a characterized allergen was the first 3 letters of genus, the first letter of species name and a number the other already characterized allergen it matched in homology and molecular weight, there were 23 known mite allergens (51).

The group 1 and 2 allergens of *Dermatophagoides* mites were clearly major specificities. About 20% of patients, however, did not have IgE antibody to the group 1 and 2 allergens, and even though this was a minority, it constituted a large population. There were also many other house dust mite allergens which had high IgE binding activity but these were presented in low and variable concentrations in mite extracts, usually at less than 1% of the group 1 and 2 allergens (111). As previously described, the trypsin enzymatic activity of Der p 3 demonstrated a 200-fold higher concentration in spent mite media as Der f 3. (103). Studies of further relevant allergens: Der p 5, 10, 11 and 14, which appeared to be present in low quantities (40). There was evidence that Der p 3, 7 and 14 were unstable in the extracts (111); nonetheless, low amounts of allergen from crude extracts induced high titres of IgE. Nonallergenic polypeptides such as the ferritin heavy chain might be highly immunogenic and induced a balanced Th1/Th2 cytokine response (30). The following recombinant allergens had been characterised: rDer f 1 (70, 128, 11, 125, 106), rDer f 2 (70, 48), rDer f 3 (96), rDer f 6 (132), rDer f 7 (88), rDer f 11 (1, 113, 114, 63, 116), rDer f 14 (28) and rDer f 16 (107).

Table 1 Molecular cloning of *Dermatophagoides* spp. allergens.

Group	Allergen	Number of amino acid residues	Deduced MW (kDa)	Potential glycosylation site(s)	Biochemical identity or homology
Group 1	Der p 1	222	24	1	Cysteine protease; homology with papain, actinidin, cathepsins B and H; sequence polymorphism
	Der f 1	223	27	1	
Group 2	Der p 2	129	15	0	NPC2 family
	Der f 2	129	15	0	
Group 3	Der p 3	232	31	0	Trypsin; homology with Der p 6 and Der f 6, mammalian and invertebrate trypsins, and other serine proteases; sequence polymorphism
	Der f 3	232	29	0	
Group 4	Der p 4	496	60	1	Amylase; homology with insect and mammalian $\alpha$ -amylases
Group 5	Der p 5	113	14	0	Function unknown; cleavage site 98 unknown
Group 6	Der p 6	231	25	0	Chymotrypsin; homology with Der p 3 and Der f 3, mammalian and invertebrate chymotrypsins, and other serine proteases
	Der f 6	230	25	0	
Group 7	Der p 7	198	26, 30, 31	1	Function unknown (25,30,31 kDa)
	Der f 7	196	30-31	1	
Group 8	Der p 8	219	27	2	GST; homology with glutathione S-transferases
Group 9	Der p 9		29		Collagenolytic serine protease
Group 10	Der p 10	284	36	0	Tropomyosin; homology with invertebrate tropomyosins
	Der f 10	284	37	0	
Group 11	Der p 11		103		Paramyosin (98 kDa); homology with invertebrate paramyosins; glycoprotein
	Der f 11		98	2	
Group 13	Der f 13				Fatty acid binding protein
Group 14	Der p 14	1650	177	0	Apolipoprotein-like protein; identity with a M-1?? allergen, &E-binding Mag1, D13961 (P39673); peptide fragments Mag1 and Mag3
	Der f 14		177		
Group 15	Der f 15	555	98/109	1	Chitinase (98/109 kDa, cDNA: 63 kDa)
Group 16	Der f 16	480	53	0	Gelsolin/villin, homology with gelsolin family
Group 17	Der f 17	284	53	4	EF-hand calcium-binding allergen
Group 18	Der f 18		60		Chitinase
Group 20	Der p 20				Arginine kinase
Group 21	Der p 21				
Group 22	Der f 22				
Group 23	Der p 23		14		Unknown function, homology to peritrophin-A domain (PF01607)

The major House dust mite Group 1 allergens Der p 1 and Der f 1 were the most potent of indoor allergens (106). Both allergens were major allergens and resulted in sensitisation in approximately 80% or greater of *D. farinae* sensitised patients (111). Although Der p 1 and Der f 1 were first isolated as cysteine proteases, some studies reported that natural Der f 1, similarly to Der p 1, exhibited mixed cysteine and serine protease activity (106). Der f 1 and Der f 2 sensitised approximately 80% to 90% of *D. farinae* sensitised individuals. Most patients (80%) appeared to have IgE antibodies to more than 1 allergen. Similarly to Der p 1 and Der p 2, Der f 1 and Der f 2 existed as a number of isoforms. Recombinant Der f 1 and rDer f 2 were highly homologous to the native forms. The Group 2 allergens induced humoral and cellular responses in 80-90% of mite-allergic individuals (43).

The Group 7 mite allergens reacted with IgE antibodies in 50% of sera from allergic patients (89). Der f 10, a tropomyosin, was a major allergen and had been shown to react with IgE antibodies in over 80% of mite-sensitised patients (2). Der f 11, a paramyosin, has been shown to be a major allergen. IgE reactivity to Der f 11 was reported for more than 80% of mite-sensitive asthmatic patients. Skin reactivity and IgE antibodies showed that 62% (13/21) and 50% (10/20) of mite sensitive asthmatic patients reacted positively with the recombinant Der f 11, respectively (114). This was similar to findings about rDer p 11, which detected IgE antibodies in a range of 41.7% to 66.7% in different allergic patient groups (63). In a preliminary study of 18 asthmatic children, 72.2% reacted positively to rDer f 11 and 88.9% showed positive reactivity to *D. farinae* extracts. Further evaluation of rDer f 11 in 24 asthmatic children who were skin test-positive to mite found that, whereas 70.8% had positive skin tests to rDer f 11, 75% had positive serum IgE reactivity to rDer f 11. Serum IgE reactivity to rDer f 11 was further investigated in a large panel of 49 mite skin test-positive asthmatic children, and similarly to before, 77.6% had positive serum IgE reactivity to rDer f 11 (114). Der f 14 has also been demonstrated to be a major allergen, detecting IgE antibodies in 65.8% of 38 sera samples from patients allergic to mites. Der f 14 is a protease-sensitive allergen. The breakdown products of this allergen provoked higher allergenic activity than did the intact allergen (40). HDMs cause allergic disease in dogs as well as humans. In geographical regions where the 2 mite species coexist, they both elicit specific IgE responses in humans, whereas dogs preferentially react to *D. farinae* extracts. In dogs,

the main IgE binding was directed to the *D. farinae* chitinase allergens Der f 15 and Der f 18, and not to the groups 1 and 2 allergens, as was found for humans. However, one study, aimed at characterising the chitinase allergens Der p 15 and Der p 18 of *D. pteronyssinus* and discovering whether they were important allergens for humans, as they were for dogs, reported that Der p 15 specific IgE was detected in 70% and Der p 18-specific IgE in 63% of a panel of 27 human allergic sera. The *D. pteronyssinus* chitinases Der p 15 and Der p 18 showed a high frequency of binding to IgE in allergic human sera. They were therefore potentially important allergens for humans as well as dogs (75). Recombinant Der f 16 protein was shown to bind IgE from mite-allergic patients at a 47% (8/17) frequency (52). Allergenic determinants in *D. farinae* were shared with other mites belonging to the *Pyroglyphidae* family and were highly cross-reactive with other *Dermatophagoides* species (100). There seems to be a limited cross-reactivity with Storage (nonpyroglyphid) mites (110). Allergen cross-reactivity had been reported between house dust mites and other invertebrates (92). In a study that investigated the individual allergens responsible for the cross-reactivity between *D. siboney* and other mite allergens in mite-allergic patients, IgE inhibition was shown to be higher with *D. farinae* (86%), *D. pteronyssinus* (54%) and *D. microceras* (49%) extracts than with *Lepidoglyphus destructor* (20%), *Tyrophagus putrescens* (11%), *Acarus siro* (18%) and *Blomia tropicalis* (6%) extracts. A diverse pattern for the individual allergens was demonstrated. The N-terminal sequences of Der s 1, 2 and 3 allergens showed higher homology to *D. farinae* and *D. microceras* than to *D. pteronyssinus*. The homology of the Group 2 allergens was higher than that of the Group 1 allergens. The individual allergens of *D. siboney* were more similar to those of *D. farinae* and *D. microceras* than to those of *D. pteronyssinus*. There was a limited and variable cross-reactivity with nonpyroglyphid mites. No single allergen was unique to *D. siboney* (34). Although a high prevalence of sensitisation occurred to the Group 1 mite allergen Blo t 1 from *Blomia tropicalis*, there was a low correlation of IgE reactivity between this allergen and the Group 1 mite allergen Der p 1 (21) and presumably Der f 1, an allergen highly homologous to Der p 1. Pso o 1 from the Sheep scab mite (*Psoroptes ovis*) displays strong homology to the Group 1 House dust mite allergens Der p 1, Der f 1 and Eur m 1 (62). Der f 7 had a predicted 213 residue polypeptide with 86% homologies to and serological cross-reactivity with Der p 7 (88).

Der f 10 was a tropomyosin. The tropomyosin of the American cockroach *Periplaneta americana* had an 80, 81 and 82% sequence identity to the tropomyosins from *D. pteronyssinus*, *D. farinae* and Shrimp, respectively, which had been previously shown to be important allergens (83). The IgE recognition by Shrimp-allergic individuals of similar amino acid sequences, homologous to Per a 1 epitopes in mite, Cockroach and Lobster tropomyosins, indicated the basis of the *in vitro* crossreactivity among invertebrate species. On the evidence of amino acid sequence similarity and epitope reactivity, Lobster tropomyosin had been shown to have the strongest and Cockroach the weakest crossreactivity with Shrimp (6). In sera of 30 patients tested and found to harbour *P. fuliginosa*-specific IgE, the IgE binding reactivity of the *P. fuliginosa* extract was inhibited as much as 79.4% by a *B. germanica* extract and as much as 63.3% by a *D. farinae* extract. The deduced amino acid sequence of cloned cDNA was identical to that of *P. americana* tropomyosin (47). Recombinant Der p 11 showed positive IgE binding reactivity in 78% of 50 *D. pteronyssinus*-sensitive asthmatic children. Der p 11, a paramyosin, had an 89% sequence identity with Der f 11 and Blo t 11 (116). A second study reported the sequence identity of Der f 11 with other known paramyosins to be 34-60% (114).

### 3. Immunity against House-dust mite allergen

#### 3.1 Antibody response

There were now 23 denominated HDM allergens or IgE binding proteins. Some could drive the sensitization while others could be bystander responses. Apart from the high IgE binding of Der p 1 and 2, it was found that 3 allergens, namely Der p 4, 5 and 7 showed 10% crossreactive antibody. Generally, IgE binding to HDMs was higher than aeroallergens. Collectively, it would appear that the Der p 1, 2, 4, 5 and 7 allergens elicited 80% of the response. The IgE binding to the other allergens was low even when the prevalence was high. It had been directly demonstrated for the group 3, 8, 10 and 20 allergens (42) and because the group 6 and 9 allergens bind even less IgE than Der p 3 (126) they were low. Only occasional people had IgE to the group 13 fatty-acid-binding-protein allergens (20) and IgE binding to the group 10 tropomyosin allergen had been shown to be low in Australia (42), USA (84) and Singapore (129). High reactivity had been found in Japan (2) and Africa (120); the geographical



inconsistency suggests a cross reactivity, which was plausible because tropomyosin had a very highly conserved amino acid sequence with 70 and 80% identity to helminth and seafood allergens (32). The IgE binding for the group 16 and 17 were also low in comparison to other allergens (51). IgG1 and IgG4 antibodies provided a comparison of Th1 and Th2 biased responses. Many reports were confirmed early studies showing that IgG antibodies to HDM extracts were predominantly found in sera with IgE antibody (68). Greatly increased IgG1 and IgG4 had been described for Der p 1 and Der p 2 as well as pan IgG anti-Der p 1 (19). IgG1 and IgG4 levels of allergic patients and healthy subjects who had been treatment with sublingual immunotherapy did not change, while specific IgE decreased significantly in both groups (7). Sera from wheezing patients and control subjects were assayed for specific IgG, IgG4 and IgE antibody to Der p. Neither IgG nor IgG4 antibody to Der p was found. Conversely, IgE antibody was strongly associated with wheezing (31). IgG1 and IgG4 antibody titers of allergic and non-allergic children to Der p 2 were more difficult to reconcile (95). Overall the IgG1 and IgG4 antibody responses show that allergic people induced Th1 and Th2 responses and both were higher than in non-allergic subjects. A comparison of IgG responses to a range of purified HDM allergens showed that both IgG1 and IgG4 antibodies were associated with the ability of the allergens to induce IgE (42). Der p 1 and 2 frequently bound both subclasses, the mid potency Der p 4, 5 and 7 bound them to a lesser degree, and the weak allergens had little activity. Studies with Western blotting also failed to reveal consistent IgG-binding components other than the major allergens (69). A caveat of the antibody binding results was other important allergens may exist. Binding of apolipoprotein (group 14) and paramyosin (group 11) to IgE from sera of Japanese and Taiwanese population with high frequency and potency, respectively (40, 116). Both these allergens were labile in extracts and difficult to produce as recombinant proteins. Other potential major allergens were the group 15 and 18 chitinase allergens that were the most important allergens for dogs. The frequency of binding of recombinant chitinase polypeptides was 60-70% (75), which was high but quantitative measurements had yet to be accomplished.

### **3.2 T-Cell Response**

T cell cloning had provided definitive evidence that non-allergic subjects make T cell responses to HDM allergens (74). Some reports had shown that PBMC

from allergic and non-allergic subjects proliferate equally well to HDM extracts or major allergens (8) but most had shown that PBMC from allergic subjects produce higher responses to HDM extracts (72). The increased proliferation had also been demonstrated for the major allergens Der p 1, Der p 2 (73), Der f 1 (16) and Der f 2 (17). An early study reported that Der p 1 could not stimulate proliferation of T cells from HDM-allergic asthmatics, but it was inconsistent with contemporary evidence including studies from the same laboratory (91). The precursor frequencies of T cells responding to defined allergens had not been examined, but extracts had been studied. Limiting dilution assays had reported frequencies of 0.05% in mite allergic and 0.01% for non-allergic subjects (81); 0.02% in both allergic and non-allergic; 0.01% for non-allergic and 0.04-0.09% for allergic subjects (12) and 0.2 and 0.8% (53). Limiting dilution analyses of exotic antigens in naive people show frequencies of 0.001% and the frequencies found after vaccinations were about 0.02% (6). By comparison it must be concluded that the anti-HDM precursor frequencies were high even in the non-allergic people. Similar high frequencies had been found for responses to birch and grass pollen allergens (4). Anti-HDM reactive T cell clones provided some of the first evidence that Th1 and Th2 cytokine polarization occurred in humans. However, it was now known that HDM allergens induced similar quantities of IFN- $\gamma$  from the PBMC of allergic and non-allergic subjects. The cloning probably showed the strong in vitro polarizing activity of IL-4 produced by cells from allergic but not non-allergic subjects.

It was reported that low dose induced Th1 more than Th2 cytokine; in contrast, high doses induced Th2 more than Th1 cytokines. The induction of IFN- $\gamma$  had been demonstrated with purified Der p 1 and Der p 2 allergens as well as extracts. Similar findings for IFN- $\gamma$  release had also been found for pollen allergens, but it was possible that the IFN- $\gamma$  was reduced in severe longterm allergy (64). There was little definitive data on the T cell responses elicited by purified allergens other than the major groups 1 and 2. Specific immunotherapy of Der p 1 to HDM in rhinitis and asthma patients and healthy subjects were observed. In healthy subjects, Der p 1 suppressed specific T cell. In patients, Der p1 suppressed proliferative T cell and Th1 (IFN-gamma) and Th2 (IL-5, IL-13) cytokine responses (49). It was showed that Der p 7 isolated from mite extracts induced similar responses to Der p 1 (88). Proliferative responses of PBMC to group 14 allergens had been shown to be similar to those

induced by major allergens by two research groups (28). The group 14 allergens had been difficult to produce or purify in the quantities required for T cell studies, so the studies had been limited to stimulation by peptides. Studies with extracts had also shown that T cell responses to antigens other than groups 1 and 2 allergens could be high (56).

#### **4. Laboratory diagnosis of allergic diseases**

Either monoclonal or polyclonal antibody has been used to measure mite allergens in the dust extract. More or less modified ELISA assays has been developed, using purified allergen or mite-allergen extracts with known, quantified amounts of allergen as standards. Monoclonal antibodies recognized just one epitope, which could be present on all isoforms of the allergen to be measured, or only on some of them; whereas polyclonal antibody recognized all epitopes/isoforms. The content of the major allergen of the mite *Dermatophagoides siboney*, Der s 1, of different batches of *D. siboney* extracts assayed with monoclonals directed against Der s 1 differed unpredictably between batches from values obtained with a kit for determination of the highly cross-reactive mite allergen Der f 1 for estimation of the content of Der s 1. Sometimes the Der f 1 kit gave higher values than the Der s 1 kit, probably because of varying isoallergen recognition. Thus, one must consider that different monoclonals did not give the same result. The data obtained were not absolute, nor universally valid. Furthermore, the method of purification of the major allergen used as standard was important. If affinity chromatography with monoclonal antibody was used to purify the major allergen used as standard, only a few isoallergens may be purified, and the standard curve would depend not on the total amount of the allergen, but on the presence of those isoforms. Therefore, the use of polyclonal antibody in these assays was an advantage (33).

##### **4.1 In vivo**

The skin prick test (SPT) was first described by Blackley in 1873 as a means of demonstrating pollen sensitization (108). This was a safe, practical and highly patient- and parent-acceptable way to look at allergen sensitivity in infants and children. A small amount of standardized allergen was introduced epicutaneously, using a standard single- or double-tined lancet. It was important note that it was no longer

accepted practice to use a small-gauge hypodermic needle, or to use a single lancet for multiple allergens (10). Allergen cross-bridging of IgE fixed on mast cells resulted in release of vasoactive histamine and other mediators of inflammation. Within 10 min a palpable itchy ‘urticarial’ papule or wheal appeared, not unlike a mosquito bite. The wheal was measured using a ruler, and recorded either as a mean of two perpendicular diameters (recorded in mm) or as an area, using a computerlinked laser reader. The older practice of comparing the wheal size to that of response to the histamine control was no longer supported, as clinicians could now use absolute wheal size expressed in mm to predict clinical reactivity, as assessed in a food challenge (104). However, it was still important to always use a histamine positive control, to ensure that the child was actually able to mount a wheal and flare response (thereby validating any wheal response that was elicited by an allergen) and was not taking an anti-histamine, which would block such a response. A negative (saline) control was always used to ensure that the child did not have dermographism or pressure sensitivity. The SPT was undertaken in infants and young children and noted for its safety and acceptability. It could be performed in low-risk children in home or school settings (102). Most adverse reactions to SPT occur in subjects with unstable allergic conditions, particularly inhalant allergen-associated asthma. These children were identifiable by history and should had SPT performed in a hospital setting (24). In older children and adults the volar (palmar) aspect of the forearm(s) was used; in infants the back was the best, as the infant could be held and comforted against a parent or assistant. Allergen SPT was difficult if there was widespread eczema. It was said to be unreliable soon after an anaphylactic episode (when the mast cells had all degranulated and require “re-stocking” (87). Apart from anti-histamines, common drugs had little effect and oral steroids and topical calcineurin inhibitors for eczema such as tacrolimus appear to have no adverse effect.

#### **4.2 In vitro**

It had been reported that specific IgE and IgG subclass antibodies against whole body antigen and two major allergens of *Dermatophagoides farinae* (Der f 1 and Der f 2) were measured in sera from 66 adults with asthma and 34 normal subjects by ELISA. The mean optical density (OD) values of specific IgE and IgG subclass antibodies in 100 studied sera were significantly higher than those of the two major allergens ( $p < 0.001$ ) and the level of Der f 2- IgG1, IgG4 and IgE were higher

than those of Der f 2 but IgG2 of Der f 1 was higher than that of Der f 2 ( $p < 0.001$ ). Among IgG subclass antibodies of Der f 1, IgG2 was significantly higher in the nonatopic group than in the atopic group. Among IgG subclass antibodies of Der f 2, IgG2 and IgG4 were significantly higher in the atopic group than in the nonatopic group (45).

The presence of IgE, IgG1 and IgG4 to concanavalin A-binding antigens (Bt-Con-A) isolated from *Blomia tropicalis* (Bt)-total extract in sera of allergic and non-allergic subjects were evaluated by sodium dodecyl sulfate polyacrylamide gel electrophoresis (SDS-PAGE) and ELISA in sera of 121 patients with allergic rhinitis and 36 non-allergic individuals. All subjects were skin prick tested with Bt-total extract and inhibition tests were performed for IgE, IgG1 and IgG4 using both extracts (Bt-total and Bt-Con-A). Skin prick test showed that 58% of the patients were sensitized to Bt (Bt+), with 52% reactive to both mites (Bt and Dp) and 6% to Bt only. ELISA showed a similar profile of IgE, IgG1 and IgG4 levels in response to Bt-total and Bt-Con-A extracts in different groups, although Bt+ patients showed a lower IgG4 reactivity to Bt-Con-A extract. Specific IgG1 levels were higher in Bt+ patients than in control subjects, and IgG4 levels showed no significant difference among groups. ELISA inhibition showed a partial IgE and total IgG1 and IgG4 cross-reactivity with *D. pteronyssinus* extract for Bt-total and Bt-Con-A extracts (3). From previous study, it was shown that ELISA was rapid, simple and specific technique for determination of specific IgE to house dust mite, although it was less sensitive than skin prick test. However, development of more sensitive assays was essential to enable the quantification of the minute amount of specific allergen present in the crude extract and the environment.

After europium (Eu) chelates were developed as labels in the 1980s (94), TR-IFMA had been reported as an ideal immunoassay technique. Time-resolved immunofluorometric assays (TR-IFMA) had been reported as an ideal immunoassay technique. Sensitivity was higher with this technique than with methods based on tritiated tracers or enzyme-conjugated tracers. In addition, TR-IFMA offers an alternative, challenging immunoassays based on  $^{125}\text{I}$  labels with the advantage of a stable, non-radioactive tracer (37). Fluorescence of the  $\text{Eu}^{3+}$  tracer was long-lived and allows for the differentiation of the short-lived background fluorescences of biological

material, plastics and optics (98). The highly specific activity of the label increases the sensitivity of immunoassays while minimizing non-specific binding of the labelled bioaffinity molecule. Other favourable features of  $\text{Eu}^{3+}$  complexes had been reviewed (25, 26, 55). Recently, TR-IFMA was developed to measure Plasma vascular endothelial growth factor (VEGF) concentrate in 92 healthy controls, in 36 benign stomach disease patients and in 92 gastric cancer patients before surgery. A standard curve for VEGF TR-IFMA had been developed with good sensitivity (0.37 pg/ml). Accuracy studies, specificity, parallelism and precision data were determined and all were found to be satisfactory. The validity of the VEGF assay was confirmed by the good correlation between the results obtained by TR-IFMA and ELISA (ELISA result =  $1.862 + 0.953$  (TR-IFMA result),  $r = 0.944$ ). At the cut-off of 217.79 pg/ml, the diagnostic sensitivity, specificity and accuracy of the TR-IFMA were 40.2, 93.7 and 69.9%, respectively (90). Moreover, time-resolved fluorescent resonance energy transfer (TR-FRET) assay was evaluated with a panel of serum samples from infected ( $n = 73$ ) and uninfected ( $n = 480$ ) sources of Brucellosis and compared to the performance of the parent cELISA, an indirect ELISA (iELISA) and fluorescence polarization assay (FPA). The performance of the TR-FRET assay matched the performance of the iELISA, which had 100% diagnostic sensitivity and specificity, and surpassed the performance of the cELISA and the FPA. The results also demonstrated that the TR-FRET technique was effective with poor-quality serum samples from the field (66). In addition to TR-FRET, double-antigen sandwich time-resolved immunofluorometric assay (DAS-TR-IFMA) had been developed to detect total anti-HCV antibodies based on biotin-streptavidin interaction. For comparison, 1025 samples were analysed by the DAS-TR-IFMA and three indirect anti-HCV antibody detection methods. For samples with discordant results, PCR-ELISA and Inno-LIA were employed as supplementary assays to analyse the presence of HCV antibodies. With regard to the 1025 clinical samples, the overall concordance between the DAS-TRIFMA and the three indirect methods was 99.41, 98.93 and 98.93 % for Ortho ELISA 3.0, WAT ELISA and I-TR-IFMA, respectively. The specificity/sensitivity of the DAS-TRIFMA, Ortho HCV ELISA 3.0, WAT HCV ELISA and I-TR-IFMA were 100%/99.09%, 99.34%/98.18%, 99.23%/97.27% and 99.01%/98.18%, respectively. The DAS-TR-IFMA was able to detect HCV antibodies at a concentration about 1/10

of that detectable by Ortho HCV ELISA 3.0, WAT HCV ELISA and I-TR-IFMA. It was concluded that the DAS-TR-IFMA was a more specific and reliable method for screening anti-HCV antibodies (124).

The purpose of our study was to evaluate a rapid and convenient fluorometric method based on time resolved fluorescence of on  $\text{Eu}^{3+}$  chelate to analyze HDM-specific IgE and to compare it with the established ELISA method. We evaluated HDM-specific IgE levels in allergic patients and healthy subjects.

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

## CHAPTER III

### MATERIALS AND METHODS

#### 1. House-dust mite (HDM) allergens

Total HDM extracts of *D. farinae* (Df) and *D. pteronyssinus* (Dp) were obtained from mite cultures provided by Siriraj Dust Mite Center of Services and research, Department of Parasitology, Faculty of Medicine Siriraj Hospital, Mahidol University, Thailand.

##### 1.1 Preparation of House dust mite allergen

Briefly, mite culture was stirred in phosphate buffered saline (PBS), pH 7.4 for overnight at 4 degree Celsius (°C). The mixture was centrifuged for 20 min at 12,000xg at 4°C. The supernatant was filtered through No.1 Whatman paper and through 0.22 µ filter. The sterile mite extract was then stored frozen at -20°C (18).

Recombinant allergen group 2 of *Dermatophagoides farinae* (rDer f 2) was produced by donated from Assistant Professor Surapon Piboonpocanun from the Institute of Molecular Biosciences, Mahidol University, Thailand.

The positive transformants containing the integration of interested genes were selected for small-scaled expression, Briefly, positive transformants (rDer f 2) and plasmic vector (pPICZ) of *Pichia pastoris* (*P. pastoris*) were grown in 2 milliliters (ml) of yeast extract peptone dextrose (YPD) containing 100 µg/ml Zeocin™ at 30 °C with vigorous shaking (250 rpm) for approximately 2 days. The starter cultures were added into 5 ml of fresh buffered minimal glycerol complex medium (BMGY) and incubated at 30 °C until the absorbance of BMGY was 0.1 at optical density (OD) 600 nanometer (nm). After that, the starter culture with OD 0.1 were cultured and harvested until the absorbances at of BMGY were 5.0. The BMGY cultures were centrifuged at 10,000xg for 5 min, and the cell pellets were resuspended in buffered minimal methanol complex medium (BMMY) using 1/5 volume of the original culture volume (approximately 1 ml). To induce expression of recombinant allergens, absolute methanol was added to a final concentration of 3% v/v to the BMMY culture every 24 h. The culture media were collected after 3 day induction. The collected culture media were centrifuged



at 12,000xg in a bench-top microcentrifuge for 3 min at room temperature. The supernatant was transferred to a separate tube and were stored frozen at -20 °C until used.

### 1.2 Determination of HDM protein

Protein concentration of HDM was determined by using the BioRad Protein Assay (dye-binding assay), (BioRad, Laboratory, CA) based on the method of Bradford. For standard protein, bovine serum albumine (Sigma, Steinheim, Germany) concentration was ranged from 0.0625 to 1 mg/ml was used. Ten microliters of each HDM protein was mixed with 90 µl of acid Coomassie blue dye and incubated at room temperature. After incubation for 5 min, the mixture was measured for the OD 595 nm.

### 1.3 Characterization of HDM allergen

Characterize the protein components of the extracted antigen were prepared from *D. farinae* and *D. pteronyssinus* by using SDS-PAGE. The SDS-PAGE was using 4% stacking gel and 12.5 % resolving gel. The extracted protein had been reduced and denatured by mixing with 4X sample buffer and then boiled in a water bath at 95°C for 10 min before loading onto the gel. The protein content used to load the gel was approximately 2 µg per lane. Electrophoresis was carried out with a constant voltage of 100 volts (v) until the front dye reaches the bottom of the gel. After that, the gel was stained with Coomassie Brilliant Blue.

Proteins were firstly separated by SDS-PAGE followed by transferring the fractionated proteins to a nitrocellulose membrane as prescribed by the manufacturer with a wet blotting apparatus (Bio-Rad, USA). The blotted membrane was blocked to prevent non-specific binding of antiserum to the membrane by gently rocking overnight at 4 °C in blocking solution. The blot was then washed by shaking vigorously in washing buffer for 5 min. The washing step was performed in six times replica. The blot was then incubated with continuous shaking at room temperature for 120 min in a 1:2000 dilution of monoclonal anti-group 2 antibodies (mAb 1D8 clone, Indoor biotechnologies Ltd, Manchester, UK). After six-time washing, the membrane was incubated with biotinylated rabbit-anti mouse IgG solution (1:5000) (SouthernBiotech, Birmingham, USA) for another 60 min at room temperature. After

six-time washing, the membrane was incubated with streptavidin-AP solution (1: 2000) (KPL, USA) for another 30 min at room temperature. The membrane was then washed with the same condition and the band of specific proteins was visualized by adding BCIP/NBT 1 component substrate (KPL, USA) and incubating at room temperature with gently shaking until color was developed.

## 2. Subjects

Fifty rhinitis patients with or without intermittent or persistent, mild-to-moderate asthma with positive SPT were selected for this investigation by Dr. Nares Wongpitoon and Dr. Voravan Durongpisitkul of Department of Pediatric, Police General Hospital, and Bangkok, Thailand during October 2008 to October 2009. For the control group, 19 healthy subjects from Silpakorn University with no history of allergic diseases were included. The study was approved by the Ethics committee of the Police general Hospital and written informed consent was obtained from all participants. The allergen extract of commercial Der p (*Dermatophagoides pteronyssinus*), Der f (*D. farinae*), CR (American Cockroach), Grass (Bermuda grass pollen), Dog (Dog Epithelium), Cat (Cat pelt), Wheat, Shrimp, Feather (Chicken, Duck, Goose), M1 (*Penicillium notatum*, *Aspergillus niger*, *Drechslera*, *Cladosporium sphaerospermum*, *Alternaria*), M2 (*Curvularia*, *Fusarium*, *Aureobasidium*, *Mucor*, *Rhizopus*) were used to screen allergic patients, according to the manufacture's instructions. Histamine dihydrochloride (10 mg/ml) was used as positive control and normal saline (0.9% w/v) was used as negative control.

SPT was performed on the skin of volunteer forearm using allergen extracts as mentioned above along with positive and negative controls. Briefly, the arm was first cleaned, then a drop of Allergen extract or control solution was placed onto a marked area of skin, with a distance of 2-3 centimeter (cm) apart. A sterile No 23G needle was used to prick the skin through the allergen drop, which allowed a small amount of allergen enter the skin. Each allergen was pricked with a separate needle. Two to three minutes later, the residue fluid on the skin was carefully wiped off to avoid mixing the adjacent samples. The reaction was measured after 15 min by copying the wheal size with transparent adhesive and kept tape onto a record sheet for later analysis. All the

patients were observed for another had for any unpleasant reactions such as local itch and swelling, local rash, generalized rash or anaphylaxis.

### 3. Immunological analysis

Ten ml of venous blood was received from each individual. Blood was centrifuged at 400g for 30 min., RT. The serum was then collected and frozen at -20 °C until used

#### 3.1 Enzyme-linked immunosorbent assay (ELISA)

IgE reactivity to a panel of proteins from Df, Dp, rDer f 2 and pPICZ was determined by ELISA. Briefly, dilute each allergen in coating buffer (50 mM carbonate/bicarbonate buffer) at concentration of 1000 ng/ml. One-hundred  $\mu$ l of each allergen was coated in each well of 96-well poly polystyrene microtiter wells (Nunc™, Denmark) and incubated at 4 °C overnight. The blocking buffer was added into each well and incubated at 37 °C for 60 min. The sera at dilution of 1: 10 was added into the well and incubated at 37 °C for 120 min. Biotinylated-labeled mouse anti-human IgE antibody (SouthernBiotech, Birmingham, USA) at dilution of 1: 1000 was added into each well and incubated at 37 °C for 60 min. The plates were added with streptavidin-peroxidase solution at dilution of 1: 1000 and incubated at 37 °C for 60 min. During each step, the plates were washed with PBS-Tween20 for 5 times. The color reaction was developed by adding ABTS® peroxidase substrate (KPL, USA). Absorbance of IgE antibody was measured at OD405nm with a Wallac 1420 microplate reader (Auto DELFIA Wallac 1420; Wallac, Turku, Finland).

For assay optimization. There were many parameters which influence the result in ELISA. These include antigen, antibody and conjugate concentration. Therefore, the following conditions were evaluated.

3.1.1 Evaluation of coating concentration of allergens. Different coating concentrations of allergens in coating buffer were evaluated. The protein concentrations of Df, rDer f 2 and pPICZ vary from 2.5, 5 and 10  $\mu$ g/ml.

3.1.2 Evaluation of subject's serum. One hundred microliters per well of allergen dilute to the 10  $\mu$ g/ml in coating buffer were transferred to an ELISA plate. Concentrations of antigens in dilution buffer were evaluated. The protein concentrations of Df, rDer f 2, Dp and pPICZ vary from 2.5, 5 and 10  $\mu$ g/ml.

3.1.3 Evaluation of biotinylated-labeled mouse anti-human IgE antibody. One hundred microliters per well of allergen dilute to the 10 µg/ml in coating buffer were transferred to an ELISA plate. Concentrations of antigens in dilution buffer were evaluated. The concentrations of biotinylated-labeled mouse anti-human IgE antibody vary from 1: 1000 and 1: 2000.

### **3.2 Time resolved fluoroimmunoassay (TRF)**

IgE reactivity to a panel of proteins from Df, Dp, rDer f2 and pPICZ was determined by TRF. Briefly, dilute each allergen in coating buffer (50 nM carbonate/bicarbonate buffer) at concentration of 1000 ng/ml One-hundred µl of each allergen was coated in each well of 96-well poly polystyrene microtiter wells (Nunc™, Denmark) and incubated at 4 °C overnight. The DELFIA® Assay Buffer was added into each well and incubated at 37 °C for 60 min. The sera at dilution of 1: 10 in DELFIA® Assay Buffer was added into the well and incubated at 37 °C for 120 min. Biotinylated-labeled mouse anti-human IgE antibody (SouthernBiotech, Birmingham, USA) at dilution of 1:1000 was added into each well and incubated at 37 °C for 60 min. The plates was added with DELFIA® EU-labeled Streptavidin at dilution of 1: 1000 and incubated at 37 °C for 60 min. During each step, the plates were washed with DELFIA® Wash concentrate for 5 times. The color reaction was developed by adding DELFIA® Enhancement Solution. Absorbance of IgE antibody was measured at OD615nm with a Wallac 1420 microplate reader (Auto DELFIA Wallac 1420; Wallac, Turku, Finland).

### **3.3 Sandwich enzyme-linked immuosorbent assay (sandwichELISA)**

IgE reactivity to a panel of proteins from Df, Dp, rDer f 2 and pPICZ was determined by sandwichELISA. Briefly, dilute monoclonal anti-group 2 antibodies dilution of 1:1000 in coating buffer (50 nM carbonate/bicarbonate buffer) add 100 µl was coated in each well of 96-well poly polystyrene microtiter wells (Nunc™, Denmark) and incubated at 4 °C overnight. The allergens at concentration of 1000 ng/ml was added into the well and incubated at 37 °C for 120 min. The sera at dilution of 1: 10 was added into the well and incubated at 37 °C for 120 min. Biotinylated-labeled mouse anti-human IgE antibody (SouthernBiotech, Birmingham, USA) at dilution of 1: 1000 was added into each well and incubated at 37 °C for 60 min.

The plates was added with streptavidin-peroxidase solution at dilution of 1: 1000 and incubated at 37 °C for 60 min. During each step, the plates were washed with PBS-Tween20 for 5 times. The color reaction was developed by adding ABTS<sup>®</sup> peroxidase substrate (KPL, USA). Absorbance of IgE antibody was measured at OD405nm with a Wallac 1420 microplate reader (Auto DELFIA Wallac 1420; Wallac, Turku, Finland).

### **3.4 Sandwich time resolved fluoroimmunoassay (sandwichTRF)**

IgE reactivity to a panel of proteins from Df, Dp, rDer f 2 and pPICZ was determined by sandwichTRF. Briefly, dilute monoclonal anti-group 2 antibodies dilution of 1:1000 in coating buffer (50 nM carbonate/bicarbonate buffer) add 100 µl was coated in each well of 96-well poly polystyrene microtiter wells (Nunc<sup>™</sup>, Denmark) and incubated at 4 °C overnight. The allergens at concentration of 1000 ng/ml was added into the well and incubated at 37 °C for 120 min. The sera at dilution of 1: 10 in DELFIA<sup>®</sup> Assay Buffer was added into the well and incubated at 37 °C for 120 min. Biotinylated-labeled mouse anti-human IgE antibody (SouthernBiotech, Birmingham, USA) at dilution of 1: 1000 was added into each well and incubated at 37 °C for 60 min. The plates was added with DELFIA<sup>®</sup> EU-labeled Streptavidin at dilution of 1: 1000 and incubated at 37 °C for 60 min. During each step, the plates were washed with DELFIA<sup>®</sup> Wash concentrate for 5 times. The color reaction was developed by adding DELFIA<sup>®</sup> Enhancement Solution. Absorbance of IgE antibody was measured at OD615nm with a Wallac 1420 microplate reader (Auto DELFIA Wallac 1420; Wallac, Turku, Finland).

In order to quantify specific IgE levels, serum from three highest HDM-sensitized individuals as analyzed by sandwich ELISA and sandwich TRF were analyzed by the ImmunoCAP<sup>™</sup> system (Pharmacia Diagnostic AB, Uppsala, Sweden) at the laboratory of Faculty of Medicine, Mahidol University, Bangkok, Thailand. The IgE levels in several dilutions of the reference serum were analyzed. Fifth calibrator points in two-fold dilutions ranging 0.22-3.49, 0.22-3.49 and 0.28-4.55 kilo units of aprotinin-specific antibodies per liter (kU<sub>A</sub>/l) of Df, rDer f 2 and Dp specific IgE respectively were made for use in calibrating curve of both sandwich ELISA and sandwich TRF.

#### 4. Statistic analysis

Levels of specific IgE to HDM allergens in sandwich ELISA and sandwich TRF were obtained from linear regression equation. All statistic calculations were performed using SPSS Version 13 (Chicago, IL, USA).

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

## CHAPTER IV

### RESULTS

#### 1. HDM–allergen characteristics

In the present study, HDM allergens consisted of native (Dp and Df) and recombinant (rDer f 2) allergens expressed in *P. pastoris*. For negative control, protein of pPICZ was used. The characters of HDM allergens were determined by SDS-PAGE and western blot, as shown in Figure 1. The molecular weight of native allergens (Df and Dp) were ranged from 10 to 72 kDa whereas that of rDer f 2 was 14 kDa. Molecular weight of pPICZ was not found. Additionally, molecular weight of rDer f 2 confirmed by western blot was 14 kDa.

มหาวิทยาลัยศิลปากร ส่วนวนลิขสิทธิ์

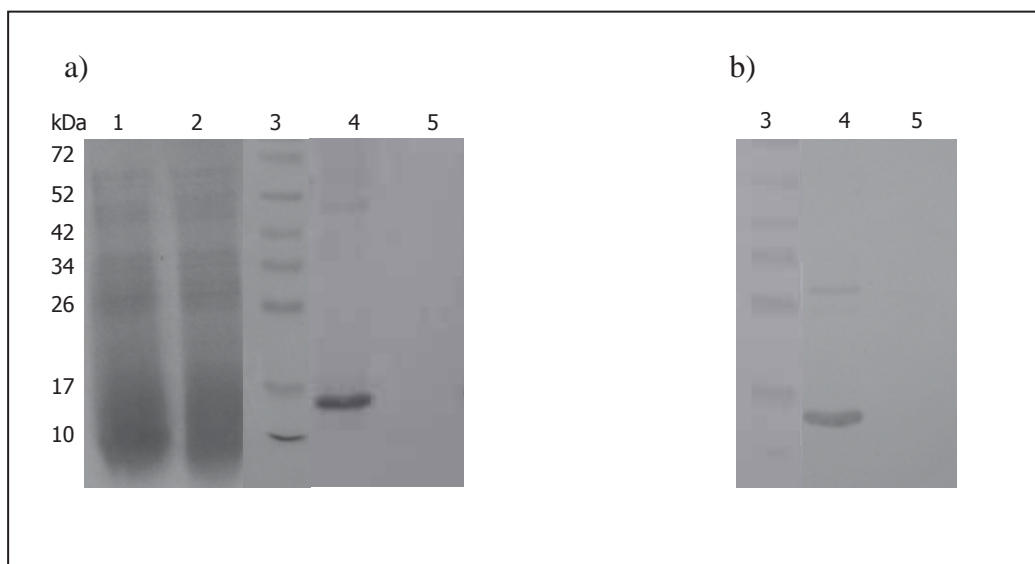


Figure 1 The protein components of HDM allergens were determined by SDS-PAGE a); Lane 1:Df; Lane 2: Dp; Lane 3: Molecular mass standards (in kDa); Lane 4: rDer f 2; Lane 5: pPICZ. b) Western blot Lane 3: Molecular mass standards (in kDa); Lane 4: rDer f 2; Lane 5: pPICZ

## 2. Subject characteristics

Specific antibodies to HDM allergens were examined in a total of 69 subjects who resided in Bangkok, Thailand (80). Subjects were screened by SPT using commercial allergens (Allertech, ALK, UK) as shown in Table 2. Histamine dihydrochloride (10 mg/ml) was used as positive control and normal saline (0.9% w/v) was used as negative control. As shown in Table 2, subjects could be divided into 2 groups; 50 allergic patients and 19 healthy subjects. The demographic clinical characteristics of these subjects were shown in Table 3 and 4.

Table 2 List of commercial allergens used for select the patient groups.

No.	Allergens	Concentrations
1.	Der f. ( <i>Dermatophagoides farinae</i> )	10,000 AU/ml
2.	Der p. ( <i>Dermatophagoides pteronyssinus</i> )	10,000 AU/ml
3.	CR (American Cockroach)	1:20 W/V
4.	Grass (Bermuda grass pollen)	10,000 BAU/ml
5.	Dog (Dog Epithelium)	15,000 PNU/ml 1:10 W/V
6.	Cat (Cat Pelt)	10,000 BAU/ml
7.	Wheat	1:10 W/V
8.	Shrimp	1:10 W/V
9.	Feather (Chicken, Duck, Goose)	1:20 W/V
10.	M1 { <i>Penicillium notatum</i> <i>Aspergillus niger</i> <i>Drechslera</i> <i>Cladosporium sphaerospermum</i> <i>Alternaria</i>	20,000 PNU/ml 1:10 W/V
11.	M2 { <i>Curruria</i> <i>Fusarium</i> <i>Aureobasidium</i> <i>Mucor</i> <i>Rhizopus</i>	20,000 PNU/ml 1:10 W/V



Table 3 Demographic and characteristics of the study individuals.

Characteristics	Groups	
	allergic individuals	healthy individuals
Number of subjects (n)	50	19
Age (years, mean $\pm$ SD)	39.52 $\pm$ 9.93	25.21 $\pm$ 6.9
Gender (male/female)	24/26	4/15
Clinical diagnosis (N, %)	50, 100 %	N/A
Categorized by allergen (%)		N/A
Der f	100 %	
Der p	100 %	
CR	20 %	
Grass	8 %	
Dog	4 %	
Cat	8 %	
Wheat	0 %	
Shrimp	0 %	
Feather	0 %	
M1	12 %	
M2	12 %	

HDM, House dust mite; Der f, *D. farinae*; Der p, *Dermatophagoides pteronyssinus*; CR, American Cockroach; Grass, Bermuda grass pollen; Dog, Dog Epithelium; Cat, Cat pelt; Wheat; Shrimp; Feather, Chicken, Duck, Goose; M1, *Penicillium notatum*, *Aspergillus niger*, *Drechslera*, *Cladosporium sphaerospermum*, *Alternaria*; M2, *Curvularia*, *Fusarium*, *Aureobasidium*, *Mucor*, *Rhizopus*





### 3. The optimization of ELISA condition for specific IgE detection

The pooled positive sera from allergic patient and negative sera from healthy subject were used as a positive and negative control for ELISA optimization.

#### 3.1 The optimization of allergen concentration

Various concentrations of Df, rDer f 2 and pPICZ (250, 500, 1000 ng/ml) were used for coating the plate. As shown in Table 5, the allergic patient specific IgE detected with Df, rDer f 2 and pPICZ were 0.133, 0.490 and 0.277 unit, respectively at OD405nm. The healthy subject specific IgE detected with Df, rDer f 2 and pPICZ were 0.133, 0.293 and 0.260 unit, respectively at OD405 nm. These results indicated that the optimal concentrations of all allergens including pPICZ were 1000 ng/ml.

#### 3.2 The optimization of serum dilution

Various dilutions of sera (1:2 and 1:10) were used for detection of specific IgE. As shown in Table 6, the allergic patient specific IgE detected with Df, rDer f 2, Dp and pPICZ were 0.185, 0.331, 0.137 and 0.144, respectively at OD405 nm. The healthy subject specific IgE detected with Df, rDer f 2, Dp and pPICZ were 0.125, 0.225, 0.122 and 0.115 unit, respectively at OD405 nm. The result indicated that the optimal dilutions for further work of sera were 1:10.

#### 3.3 The optimization of biotinylated-labeled mouse anti-human IgE antibody

Various dilutions of biotinylated-labeled mouse anti-human IgE antibody (1:1000 and 1:2000) were used for detection of soecific IgE. As shown in Table 7, the allergic patient specific IgE detected with Df, rDer f 2 and pPICZ were 0.133, 0.495 and 0.277 unit, respectively, at OD405 nm. The healthy subject specific IgE detected with Df, rDer f 2 and pPICZ were 0.133, 0.350 and 0.260 unit, respectively at OD405 nm. The result revealed that the optimal dilutions of biotinylated-labeled mouse anti-human IgE antibody for further work were 1:1000.

However, the highest concentrations of antigen detected in positive sera similar to negative sera. This indicated that coating of the well using allergen was not suitable to separate specific IgE of HDM-specific subject and healthy subject specific IgE, Sandwich ELISA using mAb was then recommended for further use.

Table 5 Optimization of Df, rDer f 2 and pPICZ concentrations for the detection of specific IgE. Various allergens concentrations (250, 500 and 1000 ng/ml) were evaluated in the experiments. The serum and biotinylated- labeled mouse anti-human IgE antibody diluted 1:10 and 1:1000, respectively by ELISA.

Subjects	Allergens concentrations (ng/ml)								
	Df			rDer f 2			pPICZ		
	250	500	1000	250	500	1000	250	500	1000
Allergic patient	0.119	0.115	0.133	0.351	0.359	0.490	0.285	0.280	0.277
Healthy subject	0.120	0.114	0.133	0.240	0.293	0.35	0.288	0.279	0.260

Table 6 Optimization of Df, rDer f 2, Dp and pPICZ concentrations for the detection of specific IgE. Allergens concentrations 1000 ng/ml was evaluated in the experiments. The biotinylated-labeled mouse anti-human IgE antibody diluted 1:1000. The serum diluted 1:2 and 1:10, respectively by ELISA.

Allergens	Serum dilution			
	Allergic patient		Healthy subject	
	1:2	1:10	1:2	1:10
Df	0.159	0.185	0.140	0.125
rDer f 2	0.199	0.331	0.240	0.255
Dp	0.148	0.137	0.123	0.122
pPICZ	0.096	0.144	0.140	0.115

Table 7 Optimization of Df, rDer f 2 and pPICZ concentrations for the detection of specific IgE. Allergens concentrations 1000 ng/ml was evaluated in the experiments. The serum diluted 1:10. The biotinylated- labeled mouse anti-human IgE antibody diluted 1:1000 and 1:2000, respectively by ELISA.

Allergens	Biotinylated-labeled mouse anti-human IgE antibody dilution			
	Allergic patient		Healthy subject	
	1:1000	1:2000	1:1000	1:2000
Df	0.133	0.108	0.133	0.144
rDer f 2	0.495	0.408	0.350	0.335
pPICZ	0.277	0.262	0.260	0.274

#### 4. Calibration curve of specific IgE detected with all HDM allergens

##### 4.1 Calibration curve between OD unit and kU<sub>A</sub>/l units

##### sandwichELISA

The calibrated line of two unit method were studied in an allergic patient who had specific IgE at 34.9 kU<sub>A</sub>/l for Df and rDer f 2 and 45.5 kU<sub>A</sub>/l for Dp compared to a healthy subject who had specific IgE at  $\leq 0.35$  kU<sub>A</sub>/l for all HDM allergens. The solid line represented the value of OD unit and kU<sub>A</sub>/l, as shown in Figure 2. In allergic patient, the highest specific IgE levels detected with Df, rDer f 2 and Dp were 3.49 kU<sub>A</sub>/l compared with 0.547 OD unit, 3.49 kU<sub>A</sub>/l compared with 0.568 OD unit and 4.55 kU<sub>A</sub>/l compared with 1.301 OD unit, respectively. The lowest specific IgE levels detected with Df, rDer f 2 and Dp were 0.22 kU<sub>A</sub>/l compared with 0.087 OD unit, 0.22 kU<sub>A</sub>/l compared with 0.085 OD unit and 0.28 kU<sub>A</sub>/l compared with 0.169 OD unit, respectively. In a healthy subject, the highest specific IgE levels after detection with all HDM allergens was less than 0.35 kU<sub>A</sub>/l compared with 0.085 OD unit. The equation of specific IgE levels in both subjects between OD unit and kU<sub>A</sub>/l unit was  $10(0.098+0.1337\text{OD unit})$  for Df,  $10(0.0921+0.1403\text{OD unit})$  for rDer f 2 and  $10(0.1579+0.2613\text{OD unit})$  for Dp.

#### **4.2 Calibration curve between counts per second (cts) and kU<sub>A</sub>/l using sandwichTRF**

The calibrated line of two unit method were also studied in the same allergic patient and the healthy subject. As shown in Figure 3, the solid line represented the values of counts compared with kU<sub>A</sub>/l. In allergic patient, the highest specific IgE levels detected with Df, rDer f 2 and Dp were with 3.49 kU<sub>A</sub>/l compared with 13456 cts, 3.49 kU<sub>A</sub>/l compared with 12549 cts and 4.55 kU<sub>A</sub>/l compared 33064 cts, respectively. The lowest specific IgE levels detected with Df, rDer f 2 and Dp were 0.22 kU<sub>A</sub>/l compared with 1327 cts, 0.22 kU<sub>A</sub>/l compared with 1311 cts and 0.28 kU<sub>A</sub>/l compared with 2789 cts, respectively. In a healthy subject, the highest specific IgE levels after detection with all HDM allergens was less than 0.35 kU<sub>A</sub>/l compared with 995 cts. The equation of specific IgE levels in both subjects between cts and kU<sub>A</sub>/l unit was 10(906+3659cts) for Df, 10(855+3399cts) for rDer f 2 and 10(1122+7178cts) for Dp.

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

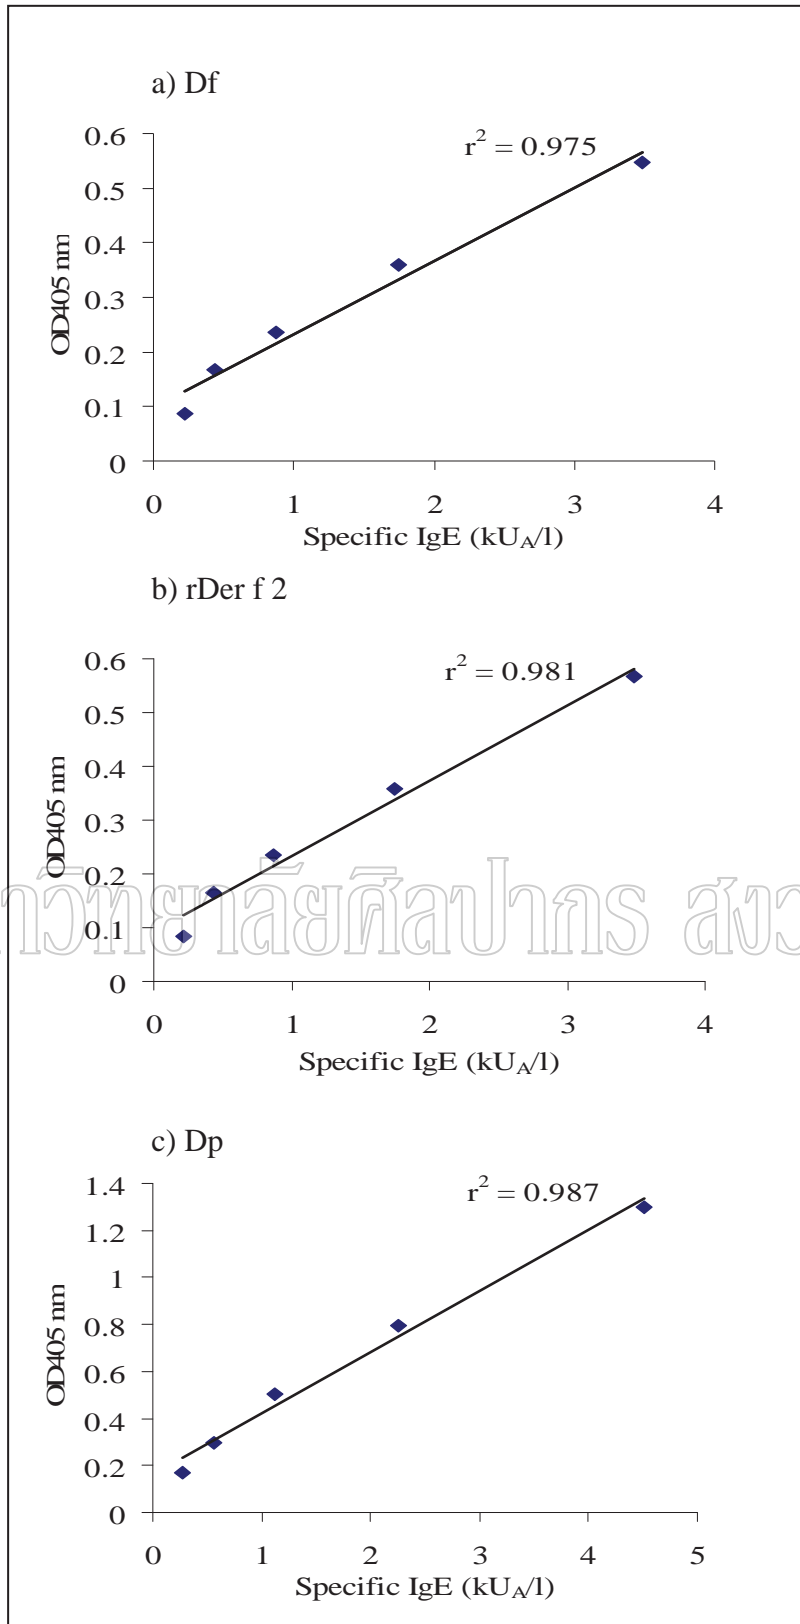


Figure 2 Calibration curve for sandwich ELISA for a) Df, b) rDer f 2 and c) Dp.



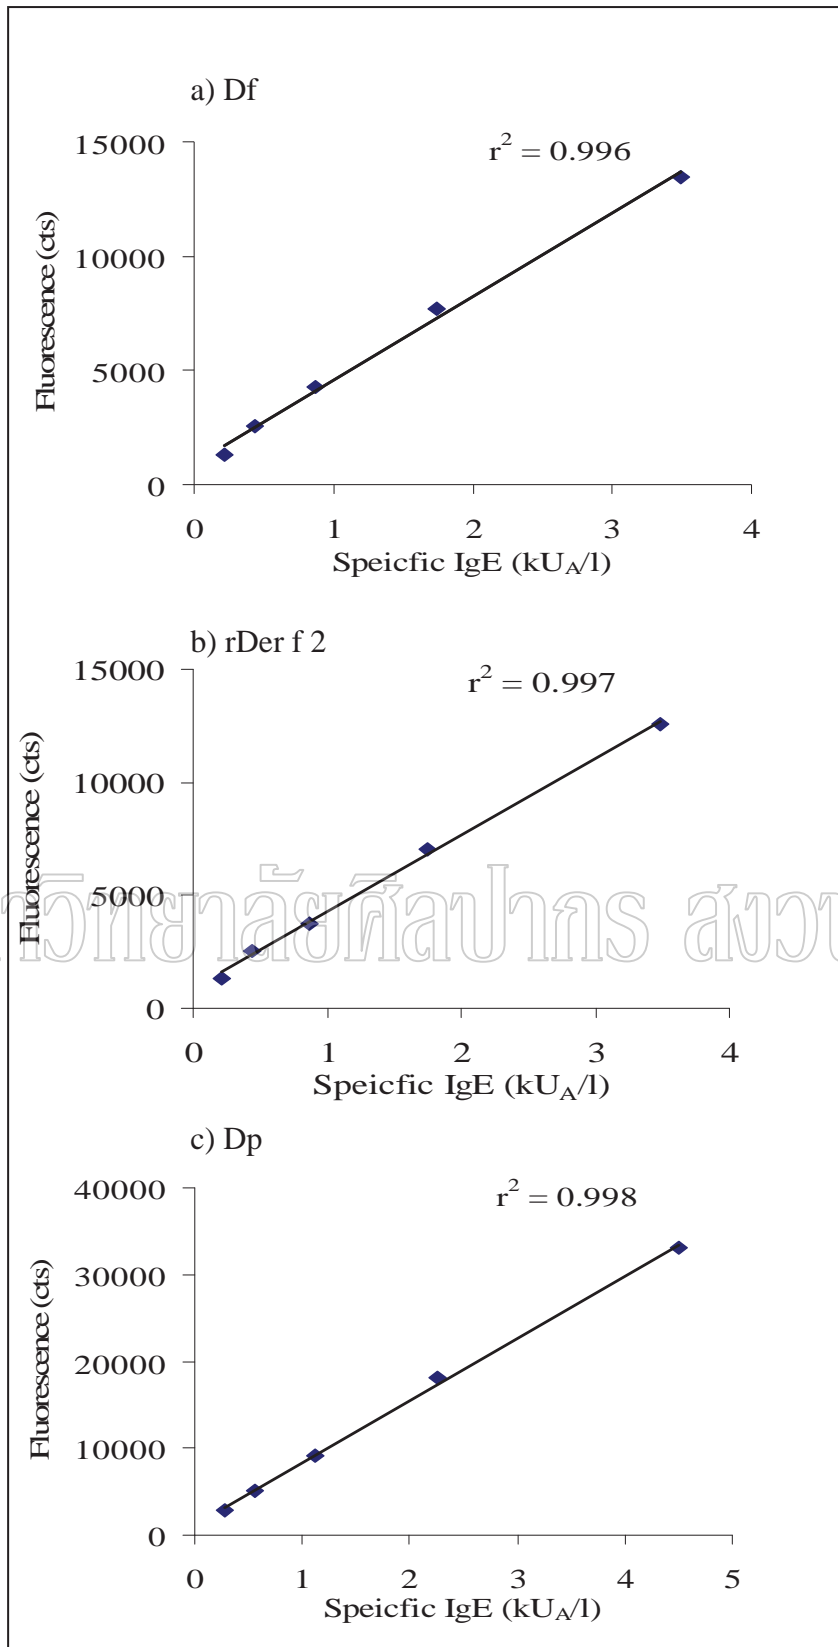


Figure 3 Calibration curve for sandwichTRF for a) Df, b) rDer f 2 and c) Dp.

## 5. Measurement of specific IgE to HDM allergens

### 5.1 Specific IgE to HDM allergens using sandwichELISA

Fifty subjects who showed allergic patients to commercial HDM and 19 healthy subjects were studied. Df, rDer f 2 and Dp allergens compared with pPICZ were used for specific IgE detection in both groups. As shown in Table 8 and 9, number of positive samples from sandwichELISA in allergic patients and healthy subject sera using Df, rDer f 2 and Dp allergen against group II mAb. Of 50 allergic patients, 13, 16 and 11 subjects showed specific IgE reactivity to Df (0.71-52.09 kU<sub>A</sub>/l), rDer f 2 (0.86-54.27 kU<sub>A</sub>/l) and Dp (3.07-76.39 kU<sub>A</sub>/l), respectively.

Of 19 healthy subjects, only one subject showed specific IgE to rDer f 2 (0.85 kU<sub>A</sub>/l). No detectable specific IgE to pPICZ was observed in sandwichELISA and sandwichTRF from all subjects.

### 5.2 Specific IgE to HDM allergens using sandwichTRF

Fifty patients who showed allergic reaction to commercial HDM and 19 healthy subjects were studied. Df, rDer f 2 and Dp allergens compared with pPICZ were used for specific IgE detection in both groups. As shown in Table 8 and 9, number of positive samples from sandwichTRF in allergic patient and healthy participant serum using Df, rDer f 2 and Dp allergen against group II mAb. Of 50 allergic patients, 31, 31 and 25 subjects showed specific IgE reactivity to Df (1.15-90.61 kU<sub>A</sub>/l), rDer f 2 (1.27-79.82 kU<sub>A</sub>/l) and Dp (0.67-106.17 kU<sub>A</sub>/l), respectively.

Of 19 healthy subjects, 5, 6 and 1 subjects showed specific IgE reactivity to Df (1.52-2.14 kU<sub>A</sub>/l), rDer f 2 (1.14-2.19 kU<sub>A</sub>/l) and Dp (1.04 kU<sub>A</sub>/l). No detectable specific IgE to pPICZ was observed in sandwichELISA and sandwichTRF from all subjects.

Number of positive samples from both methods in allergic patients and healthy subject sera using Df, rDer f 2 and Dp allergens against group II mAb were shown in Table 10. SandwichTRF detected specific IgE in higher percentage of allergic patient serum sample when tested using Df, rDer f 2 and Dp allergen (62, 62 and 50%) compared to sandwichELISA result (26, 32 and 22%). In 19 healthy subjects, sandwichELISA detected specific IgE in 0, 5.3 and 0% samples tested by the three HDM allergens while sandwichTRF found 26.3, 31.6 and 5.3% positive samples respectively.

SandwichTRF was compared to sandwichELISA by parallel testing of 50 serum specimens from rhinitis patients utilizing Df, rDer f 2 and Dp allergen respectively. Among allergic patients very good overall correlation between sandwich ELISA and sandwichTRF was found (Fig. 4). The linear regression coefficient values of Df, rDer f 2 and Dp calculated from the positive specimens varied between 0.93-0.96.

SandwichTRF positive cases from allergic patient sera tested with all HDM allergens were separated into two groups, namely those from sandwichELISA positive and sandwichELISA negative samples. Number of samples, frequency and median of each group was shown according to specific allergen in Table 11. Median, standard deviation, 25 % and 75% values were presented in Figure 5. Among sandwichTRF positive samples, 54.84 %, 48.39 % and 56 % of Df, rDer f 2, and Dp were identified as sandwichELISA negative samples.

Concentrations of HDM IgE TRF from all HDM allergens testing (allergic patients and healthy subjects) were subjected to test for several related sample using Friedman test. At  $N = 69$ ,  $p$  value equals 0.093. The use of any of the HDM allergens did not give a statistically significant result in TRF technique.

Table 8 Profiles of 50 allergic patients detected specific IgE to Df, rDer f 2, Dp and pPICZ (cut-off value=0.35 kU<sub>A</sub>/l).

ID.	Specific IgE (kU <sub>A</sub> /l)							
	sandwichELISA				sandwichTRF			
	Df	rDer f 2	Dp	pPICZ	Df	rDer f 2	Dp	pPICZ
A1	0.71	1.20	-	-	2.77	2.15	1.16	-
A2	-	-	-	-	1.15	1.48	-	-
A3	-	-	-	-	-	5.01	-	-
A4	-	0.96	-	-	1.57	2.12	-	-
A5	0.71	-	-	-	2.72	1.93	0.67	-
A6	-	-	-	-	5.56	4.17	1.64	-
A7	-	1.06	-	-	-	2.38	0.88	-
A8	-	-	-	-	1.27	2.96	1.51	-
A9	5.09	12.93	7.73	-	6.22	13.22	12.81	-
A10	-	-	-	-	1.30	3.84	1.02	-
A11	10.32	14.46	9.76	-	16.10	44.46	22.90	-
A12	-	-	-	-	1.38	1.90	-	-
A13	1.98	4.27	3.07	-	5.77	7.01	6.60	-
A14	-	-	-	-	-	-	2.50	-
A15	23.71	41.65	34.66	-	77.59	98.26	54.95	-
A16	-	-	-	-	-	-	-	-
A17	-	-	-	-	2.75	2.45	1.30	-
A18	-	-	-	-	1.81	-	-	-
A19	-	-	-	-	-	-	-	-
A20	-	-	-	-	11.00	5.80	3.68	-
A21	-	-	-	-	3.18	3.63	1.93	-
A22	-	1.13	-	-	2.57	3.96	1.67	-
A23	5.16	21.98	25.28	-	2.88	14.18	17.94	-

- = < 0.35 kU<sub>A</sub>/l

Table 8 (continue) Profiles of 50 allergic patients detected specific IgE to Df, rDer f 2, Dp and pPICZ (cut-off value=0.35 kU<sub>A</sub>/l).

ID.	Specific IgE (kU <sub>A</sub> /l)							
	sandwich ELISA				sandwich TRF			
	Df	rDer f 2	Dp	pPICZ	Df	rDer f 2	Dp	pPICZ
A24	-	-	-	-	3.52	5.42	3.07	-
A25	-	-	-	-	1.18	1.27	-	-
A26	27.64	46.75	49.76	-	10.63	30.45	46.16	-
A27	-	-	-	-	-	-	-	-
A28	34.82	45.04	69.64	-	17.54	19.15	74.92	-
A29	-	-	-	-	-	-	-	-
A30	12.49	21.63	22.39	-	26.59	27.87	28.73	-
A31	-	-	-	-	-	-	-	-
A32	6.88	6.91	29.95	-	29.85	29.82	48.95	-
A33	-	-	-	-	1.72	2.34	-	-
A34	-	-	-	-	1.16	1.77	-	-
A35	-	-	-	-	-	-	-	-
A36	-	-	-	-	-	-	-	-
A37	-	-	-	-	-	-	-	-
A38	-	-	-	-	-	-	-	-
A39	-	-	-	-	-	-	-	-
A40	-	-	-	-	-	-	-	-
A41	-	-	-	-	-	-	-	-
A42	28.05	30.53	39.58	-	38.05	32.85	37.19	-
A43	52.09	54.27	76.39	-	90.61	79.82	106.17	-
A44	-	-	-	-	-	-	-	-
A45	-	-	-	-	-	-	-	-
A46	-	-	-	-	-	-	-	-

- = < 0.35 kU<sub>A</sub>/l

Table 8 (continue) Profiles of 50 allergic patients detected specific IgE to Df, rDer f 2, Dp and pPICZ (cut-off value=0.35 kU<sub>A</sub>/l).

ID.	Specific IgE (kU <sub>A</sub> /l)							
	sandwichELISA				sandwichTRF			
	Df	rDer f 2	Dp	pPICZ	Df	rDer f 2	Dp	pPICZ
A47	-	-	-	-	-	-	-	-
A48	-	-	-	-	2.42	-	-	-
A49	-	-	-	-	2.33	2.74	6.08	-
A50	-	0.86	2.17	-	5.68	6.41	12.52	-

- = < 0.35 kU<sub>A</sub>/l

มหาวิทยาลัยศิลปากร ส่วนลิขสิทธิ์

Table 9 Profiles of 19 Healthy subjects detected specific IgE to Df, rDer f 2, Dp and pPICZ (cut-off value=0.35 kU<sub>A</sub>/l).

ID.	Specific IgE (kU <sub>A</sub> /l)							
	sandwichELISA				sandwichTRF			
	Df	rDer f 2	Dp	pPICZ	Df	rDer f 2	Dp	pPICZ
H1	-	0.85	-	-	1.52	1.55	-	-
H2	-	-	-	-	-	-	-	-
H3	-	-	-	-	-	1.50	-	-
H4	-	-	-	-	1.36	1.92	-	-
H5	-	-	-	-	1.68	-	-	-
H6	-	-	-	-	2.14	-	-	-
H7	-	-	-	-	-	1.14	-	-
H8	-	-	-	-	1.69	2.19	-	-
H9	-	-	-	-	-	-	-	-
H10	-	-	-	-	-	1.25	1.04	-
H11	-	-	-	-	-	-	-	-
H12	-	-	-	-	-	-	-	-
H13	-	-	-	-	-	-	-	-
H14	-	-	-	-	-	-	-	-
H15	-	-	-	-	-	-	-	-
H16	-	-	-	-	-	-	-	-
H17	-	-	-	-	-	-	-	-
H18	-	-	-	-	-	-	-	-
H19	-	-	-	-	-	-	-	-

- = < 0.35 kU<sub>A</sub>/l

Table 10 Number of positive samples from sandwichELISA and sandwichTRF in allergic patient and healthy participant serum as seen using Df, rDer f 2 and Dp allergens against group II mAb.

Allergen tested	Number of positive samples: n (frequency %)	
	Allergic patients Total n = 50	Healthy participants Total n = 19
<b>Df</b>		
sandwichELISA	13 (26%)	0 (0%)
sandwichTRF	31 <sup>1</sup> (62%)	5 (26.3%)
<b>rDer f 2</b>		
sandwichELISA	16 (32%)	1 (5.3%)
sandwichTRF	31 <sup>2</sup> (62%)	6 (31.6%)
<b>Dp</b>		
sandwichELISA	11 (22%)	0 (0%)
sandwichTRF	25 <sup>3</sup> (50%)	1 (5.3%)

<sup>1,2,3</sup> correspond to the same data in Table 11.

Table 11 SandwichTRF positive cases in serum from allergic patients categorized by sandwichELISA result in Df, rDer f 2 and Dp testing.

HDM allergens	sandwichTRF positive cases in symptomatic patients	
	sandwichELISA positive	sandwichELISA negative
<b>Df: total 31 samples<sup>1</sup></b>		
n (frequency %)	13 (45.16%)	17 (54.84%)
Median (kU <sub>A</sub> /l)	13.37	1.81*
<b>rDer f 2: total 31 samples<sup>2</sup></b>		
n (frequency %)	16 (51.61%)	15 (48.39%)
Median (kU <sub>A</sub> /l)	16.67	2.74*
<b>Dp: total 25 samples<sup>3</sup></b>		
n (frequency %)	11 (44%)	14 (56%)
Median (kU <sub>A</sub> /l)	37.19	1.66*

Mann-Whitney Rank Sum Test;  $p < 0.001^*$



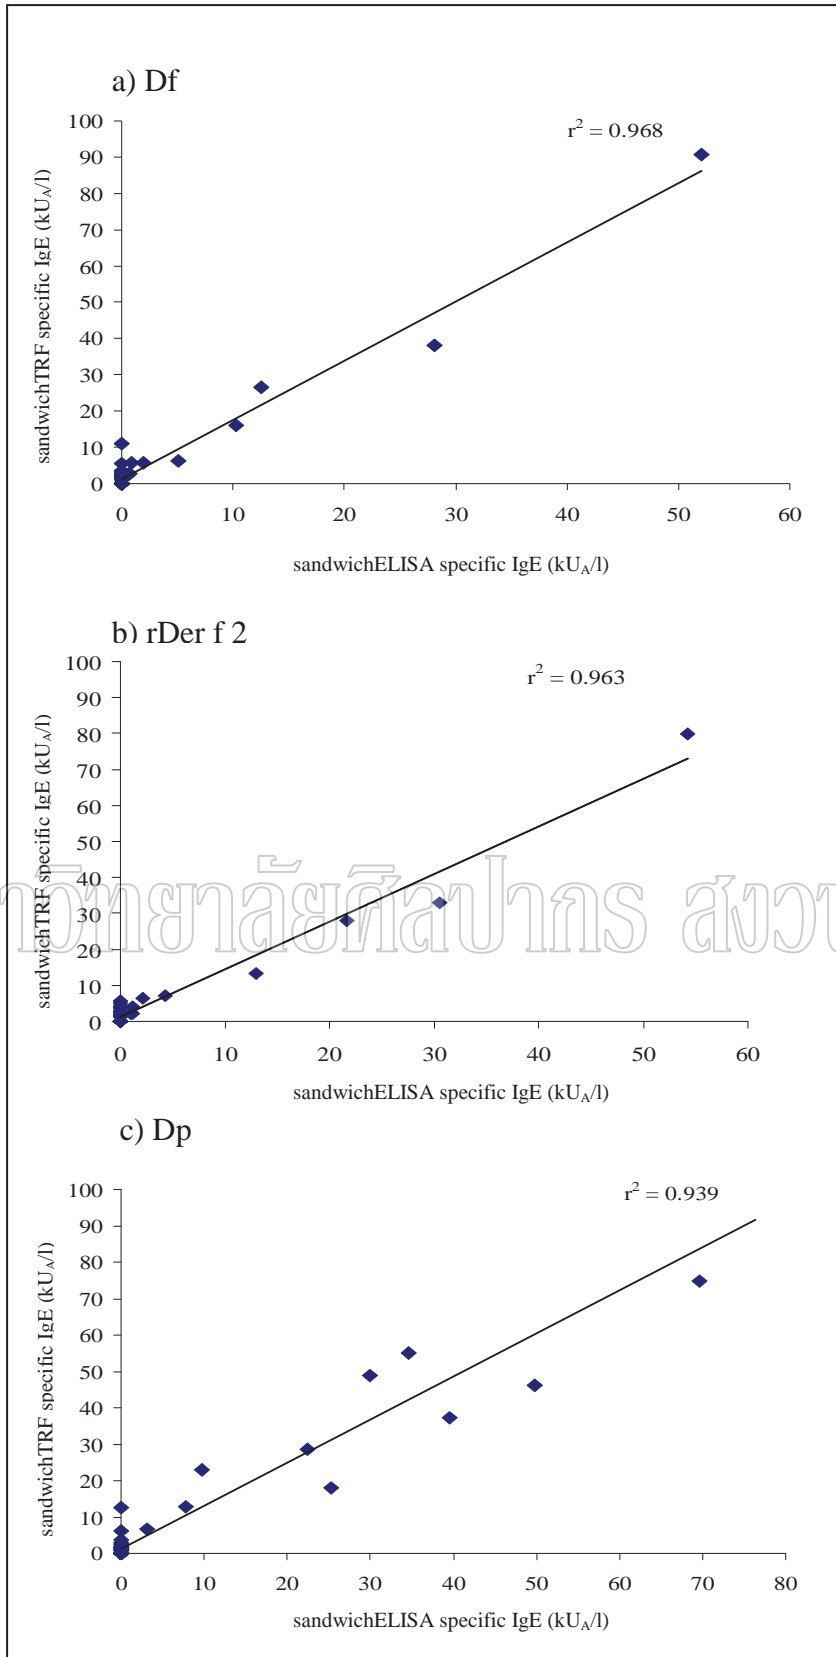


Figure 4 Correlation between levels of specific IgE against a) Df, b) rDer f 2 and c) Dp measured by sandwichELISA and sandwichTRF.

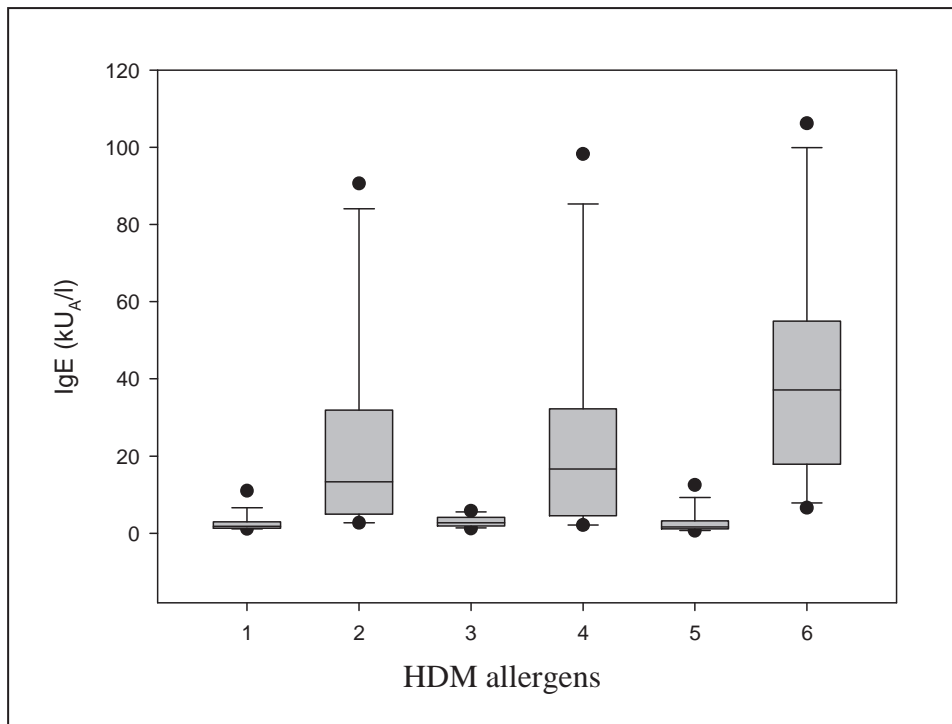


Figure 5 SandwichTRF positive cases from serum of allergic patients tested with all three HDM allergens. Median, standard deviation, 25 and 75 percent values were presented. HDM allergens, Df : 1) sandwichELISA negative, 2) sandwichELISA positive; rDer f 2 : 3) sandwichELISA negative, 4) sandwichELISA positive; Dp : 5) sandwichELISA negative, 6) sandwichELISA positive.

## CHAPTER V

### DISCUSSION

It has been reported that *D. farinae* which homologous with *D. pteronyssinus* is composed of broad range of 10 to 72 kDa. In the present study, Immunoblotting analysis of rDer f 2 using a specific group II mAb showed one band of 14 kDa (Figure 1), agreeing with previous reports Thus it is an implication that rDer f 2 corresponded to *D. farinae* (58, 78). It is known that *D. farinae* usually coexists with *D. pteronyssinus*. As a result the assay measuring IgE binding to rDer f 2 would not distinguish *D. farinae* sensitization with cross reactivity (127).

#### **Levels of specific IgE reactivity to HDM allergens: Lower detection limit and increase testing sensitivity**

The IgE reactivity profile for the sera from allergic patients (n = 50) and healthy subjects (n = 19) was determined by three different allergens, namely Df, rDer f 2 and Dp measured by TRF compared with ELISA.

As shown in Table 10, the efficacy of recombinant antigen (rDer f 2) and natural antigen (Df or Dp) were examined in allergic patients and non-allergic individuals by both TRF and ELISA. In allergic patients, we found that only 26 %, 32 % and 22 % result was obtained by ELISA, while 62 %, 62 % and 50 % of patient sera reacted with Df, rDerf2, and Dp respectively using TRF. The increase in rate of HDM IgE detection was significant at 34 %, 30 % and 28 % for all three allergen, respectively. This is the first indication suggesting that TRF of all three HDM allergens show higher sensitivity for serum of people with allergic symptoms with no detectable HDM IgE. In addition, when ELISA showed 0 %, 5.3 % and 0 % positive samples in healthy sera, TRF detected 26.3 %, 31.6 % and 5.3 % positive samples. That is the 26.3 %, 21.3 % and 5.3 % higher detection rate across the board.

In 50 HDM-SPT positive allergic subjects, 48 percents of this group showed cross-reactive IgE binding to all three allergens measured by TRF, while only 22 percent showed cross-reactive IgE binding to all three allergens measured by ELISA. Additionally, cross-reactive IgE to two allergens was also observed by both TRF and

ELISA. TRF showed 10 %, 2 % and 0 % cross-reactivity between Df/rDer f 2, rDer f 2/Dp and Df/Dp, while ELISA result showed 2 %, 0 % and 0 %, respectively. In healthy participants there was no cross-reactivity report over all three antigens. Only 15.8 and 5.3 percent cross-reactivity were reported for Df/rDer f 2 and rDer f 2/Dp. These numbers confirms TRF sensitivity over ELISA and suggests that rDerf2 is a slightly better antigen as seen from cross-reactivity data.

Table 11 and Figure 5 revealed lower detection limit and the sensitivity of TRF. All HDM allergens provided significantly different median between ELISA positive and negative samples in Mann-Whitney Rank Sum Test with  $p < 0.001$ . Figure 5 showed that even though ranges of all three ELISA negative groups showed overlap with the ELISA positive ones, one hundred percent of all three ELISA negative populations stayed within 40 percentile of the corresponding ELISA positive population. TRF was able to show real value of some ELISA negative samples beautifully in this demonstration. This investigation employed three different HDM allergens, namely Df and Dp from natural sources, and a recombinant rDer f 2. Result from the test for several related samples using Friedman test showed that TRF results using all three allergens were not significantly different from another. Thus this investigation suggested that rDer f 2 can be used as a HDM allergen in TRF. Since rDer f 2 has been expressed in large quantity, this should ensure a homogeneous batch supply of HDM allergen for time to come. Immunoassays based on time-resolved fluorometry represented an attractive option that offers several advantages over other traditional techniques, including very high sensitivity, no use of radioactive reagents, stability of the reagents, low background interference and a wide test range (76, 131). Additionally, the use of a specific mAb as capture antibody in this study avoided over estimation of allergens by reducing the cross-reactive epitopes recognition. The use of specific polyclonal serum avoided the loss of detection produced by conformational changes affecting one or more epitopes. Hence, a specific anti-HDM polyclonal serum has been used as the secondary antibody in this investigation, unlike most of other immunoassays described (33).

The time-resolved immunofluorometric assay developed in this investigation provided sensitive and highly specific techniques for the determination of HDMspecific IgE in human sera. Measurements achieved with TRF and ELISA were

highly correlated ( $r^2$  between 0.93-0.96). In regard to the limit of detection, the assay allowed the detection of HDM-specific IgE as low as  $< 0.35$  kUA/l, which was well below limits of detection reported by other techniques, namely Immunoblot, ELISA, and RIA. TRF could therefore be considered the most sensitive method for quantifying HDM-specific IgE. In addition, the assay range of TRF was larger than that of conventional ELISA in our laboratory. This finding was consistent with previous reports (124, 90). It is clearly seen that TRF showed sensitivity to serum of allergic patients with symptom whose serum were formerly HDM IgE negative using ELISA. TRF showed IgE detection in real samples from ELISA HDM positive allergic patients. TRF was also capable of detecting IgE in ELISA HDM negative but positive to SPT aeroallergens. It is thus demonstrated that a broad range of HDM-specific IgE could be detected with the TRF.

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

## CHAPTER VI

### CONCLUSION

TRF was developed for HDM allergen IgE testing and evaluated. Such improvements may be useful for screening of HDM allergy and other aeroallergens. TRF of Df, rDer f 2 and Dp showed lower detection limit than ELISA and yielded higher sensitivity for serum of people with allergic symptoms with no detectable HDM IgE. Recombinant HDM allergen, rDer f 2, was proven to be as good an allergen as its natural counterpart, namely Df and Dp. It is anticipated that TRF for HDM-specific IgE detection will play an important role in future diagnosis of HDM allergy in clinical laboratories and for different research purposes.

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

## REFERENCE

1. Aki T, Fujikawa A, Wada T, Jyo T, Shigeta S, Murooka Y, et al. Cloning and expression of cDNA coding for a new allergen from the house dust mite, *Dermatophagoides farinae*: homology with human heat shock cognate proteins in the heat shock protein 70 family. *J Biochem.* 1994;115(3):435-40.
2. Aki T, Kodama T, Fujikawa A, Miura K, Shigeta S, Wada T, et al. Immunochemical characterization of recombinant and native tropomyosins as a new allergen from the house dust mite, *Dermatophagoides farinae*. *J Allergy Clin Immunol.* 1995;96(1):74-83.
3. Almeida KC, Silva DA, Gennari-Cardoso ML, Cunha-Júnior JP, Alves R, Ynoue LH, et al. Responses of IgE, IgG1, and IgG4 to concanavalin A-binding *Blomia tropicalis* antigens in allergic patients. *Braz J Med Biol Res.* 2006;39(11):1445-54.
4. Assing K, Nielsen CH, Poulsen LK. Immunological characteristics of subjects with asymptomatic skin sensitization to birch and grass pollen. *Clin Exp Allergy.* 2006;36(3):283-92.
5. Avanzini MA, Belloni C, Soncini R, Ciardelli L, de Silvestri A, Pistorio A, et al. Increment of recombinant hepatitis B surface antigen-specific T-cell precursors after revaccination of slow responder children. *Vaccine.* 2001;19(20-22):2819-24.
6. Ayuso R, Reese G, Leong-Kee S, Plante M, Lehrer SB. Molecular basis of arthropod cross-reactivity: IgE-binding cross-reactive epitopes of shrimp, house dust mite and cockroach tropomyosins. *Int Arch Allergy Immunol.* 2002;129(1):38-48.
7. Bahceciler NN, Arıkan C, Taylor A, Akdis M, Blaser K, Barlan IB, et al. Impact of sublingual immunotherapy on specific antibody levels in asthmatic children allergic to house dust mites. *Int Arch Allergy Immunol.* 2005;136(3):287-94.
8. Bellinghausen I, Brand U, Knop J, Saloga J. Comparison of allergen-stimulated dendritic cells from atopic and nonatopic donors dissecting their effect

- on autologous naive and memory T helper cells of such donors. *J Allergy Clin Immunol.* 2000;105(5):988-96.
9. Bergmann RL, Edenharter G, Bergmann KE, Lau S, Wahn U. Socioeconomic status is a risk factor for allergy in parents but not in their children. *Clin Exp Allergy.* 2000;30(12):1740-5.
  10. Bernstein IL, Storms WW. Practice parameters for allergy diagnostic testing. Joint Task Force on Practice Parameters for the Diagnosis and Treatment of Asthma. The American Academy of Allergy, Asthma and Immunology and the American College of Allergy, Asthma and Immunology. *Ann Allergy Asthma Immunol.* 1995;75(6 Pt 2):543-625.
  11. Best EA, Stedman KE, Bozic CM, Hunter SW, Vailes L, Chapman MD, et al. A recombinant group 1 house dust mite allergen, rDer f 1, with biological activities similar to those of the native allergen. *Protein Expr Purif.* 2000;20(3):462-71.
  12. Burastero SE, Fenoglio D, Crimi E, Brusasco V, Rossi GA. Frequency of allergen-specific T lymphocytes in blood and bronchial response to allergen in asthma. *J Allergy Clin Immunol.* 1993;91(5):1075-81.
  13. Burney P, Malmberg E, Chinn S, Jarvis D, Luczynska C, Lai E. The distribution of total and specific serum IgE in the European Community Respiratory Health Survey. *J Allergy Clin Immunol.* 1997;99(3):314-22.
  14. Bush R, Wood R, Eggleston P. Laboratory animal allergy. *J Allergy Clin Immunol.* 1998;102(1):99-112.
  15. Calvo M, Fernandez-Caldas E, Arellano P, Marin F, Carnes J, Hormaechea A. Mite allergen exposure, sensitisation and clinical symptoms in Valdivia, Chile. *J Investig Allergol Clin Immunol.* 2005;15(3):189-96.
  16. Cavaillon JM, Fitting C, Guinnepain MT, Rassemont R, David B. Lymphocyte proliferative responses to the purified *Dermatophagoides farinae* major allergen in untreated and hyposensitized atopic patients. *Allergy.* 1988;43(2):146-51.
  17. Chao PL, Peng HJ, Tang RB, Hung MW, Tsai LC. Serum specific IgE reactivity to recombinant Der f 11 in asthmatic children. *J Asthma.* 2001;38(5):391-8.



18. Chapman MD, Heymann PW, Wilkins SR, Brown MJ, Platts-Mills TA. Monoclonal immunoassays for major dust mite (*Dermatophagoides*) allergens, Der p I and Der f I, and quantitative analysis of the allergen content of mite and house dust extracts. *J Allergy Clin Immunol.* 1987;80(2):184-94.
19. Chapman MD, Platts-Mills TA. Measurement of IgG, IgA and IgE antibodies to *Dermatophagoides pteronyssinus* by antigen-binding assay, using a partially purified fraction of mite extract (F4P1). *Clin Exp Immunol.* 1978;34(1):126-36.
20. Chan SL, Ong ST, Ong SY, Chew FT, Mok YK. Nuclear magnetic resonance structure-based epitope mapping and modulation of dust mite group 13 allergen as a hypoallergen. *J Immunol.* 2006;176(8):4852-60.
21. Cheong N, Soon SC, Ramos JD, Kuo IC, Kolatkar PR, Lee BW, et al. Lack of human IgE cross-reactivity between mite allergens Blo t 1 and Der p 1. *Allergy.* 2003;58(9):912-20.
22. Chiang CH, Wu KM, Wu CP, Yan HC, Perng WC. Evaluation of risk factors for asthma in Taipei City. *J Chin Med Assoc.* 2005;68(5):204-9.
23. Christopher Maple PA, Jones CS. Time-resolved fluorometric immunoassay for rubella antibody-a useful method for serosurveillance studies. *Vaccine.* 2002;20(9-10):1378-82.
24. Devenney I, Falth-Magnusson K. Skin prick tests may give generalized allergic reactions in infants. *Ann Allergy Asthma Immunol.* 2000;85(6 Pt 1):457-60.
25. Diamandis EP. Immunoassays with time-resolved fluorescence spectroscopy: principles and applications. *Clin Biochem.* 1988;21(3):139-50.
26. Dickson EF, Pollak A, Diamandis EP. Ultrasensitive bioanalytical assays using time-resolved fluorescence detection. *Pharmacol Ther.* 1995;66(2):207-35.
27. El-Shazly AM, El-Beshbishi SN, Azab MS, El- Nahas HA, Soliman ME, Fouad MA, Monib Mel. Present situation of house dust mites in Dakahlia Governorate, Egypt. *J Egypt Soc Parasitol.* 2006; 36(1):113-26.

28. Epton MJ, Dilworth RJ, Smith W, Thomas WR. Sensitisation to the lipid-binding apolipoprotein allergen Der p 14 and the peptide Mag-1. *Int Arch Allergy Immunol.* 2001;124(1-3):57-60.
29. Epton MJ, Dilworth RJ, Smith W, Hart BJ, Thomas WR. High-molecular-weight allergens of the house dust mite: an apolipoprotein-like cDNA has sequence identity with the major M-177 allergen and the IgE-binding peptide fragments Mag1 and Mag3. *Int Arch Allergy Immunol.* 1999;120(3):185-91.
30. Epton MJ, Smith W, Hales BJ, Hazell L, Thompson PJ, Thomas WR. Non-allergenic antigen in allergic sensitization: responses to the mite ferritin heavy chain antigen by allergic and non-allergic subjects. *Clin Exp Allergy.* 2002;32(9):1341-7.
31. Erwin EA, Wickens K, Custis NJ, Siebers R, Woodfolk J, Barry D, et al. Cat and dust mite sensitivity and tolerance in relation to wheezing among children raised with high exposure to both allergens. *J Allergy Clin Immunol.* 2005;115(1):74-9.
32. Fernandes J, Reshef A, Patton L, Ayuso R, Reese G, Lehrer SB. Immunoglobulin E antibody reactivity to the major shrimp allergen, tropomyosin, in unexposed Orthodox Jews. *Clin Exp Allergy.* 2003;33(7):956-61.
33. Ferrandiz R, Casas R, Dreborg S, Einarsson R, Fernandez B. Crossreactivity between *Dermatophagoides siboney* and other house dust mite allergens in sensitized asthmatic patients. *Clin Exp Allergy.* 1995;25(10):929-34.
34. Ferrandiz R, Casas R, Dreborg S. Cross-reactivity between *Dermatophagoides siboney* and other domestic mites. II. Analysis of individual cross-reacting allergens after SDS-PAGE and Western blotting inhibition. *Int Arch Allergy Immunol.* 1998;116(3):206-14.
35. Ferrandiz R, Casas R, Dreborg S. Purification and IgE binding capacity of Der s 3, a major allergen from *Dermatophagoides siboney*. *Clin Exp Allergy.* 1997;27(6):700-4.
36. Ferrandiz R, Casas R, Dreborg S, Einarsson R, Bonachea I, Chapman M. Characterization of allergenic components from house dust mite

- Dermatophagoides siboney. Purification of Der s 1 and Der s 2 allergens. Clin Exp Allergy. 1995;25(10):922-8.
37. Fiet J, Giton F, Fidaa I, Valleix A, Galons H, Raynaud JP. Development of a highly sensitive and specific new testosterone time-resolved fluoroimmunoassay in human serum. Steroids. 2004;69(7):461-71.
  38. Fujii S, Ono K, Shigeta S, Jyo T, Yamashita U. Human T cell responses to recombinant mite antigens of Dermatophagoides farinae. Clin Exp Immunol. 1997;108(2):284-8.
  39. Fujikawa A, Ishimaru N, Seto A, Yamada H, Aki T, Shigeta S, et al. Cloning and characterization of a new allergen, Mag 3, from the house dust mite, Dermatophagoides farinae: cross-reactivity with high-molecular-weight allergen. Mol Immunol. 1996;33(3):311-9.
  40. Fujikawa A, Uchida K, Yanagidani A, Kawamoto S, Aki T, Shigeta S, et al. Altered antigenicity of M-177, a 177-kDa allergen from the house dust mite Dermatophagoides farinae, in stored extract. Clin Exp Allergy. 1998;28(12):1549-58.
  41. Gulegen E, Girisgin O, Kutukoglu F, Girisgin AO, Coskun SZ. Mite species found in house dust in houses in Bursa. Turkiye Parazitol Derg. 2005;29(3):185-7.
  42. Hales BJ, Martin AC, Pearce LJ, Laing IA, Hayden CM, Goldblatt J, et al. IgE and IgG anti-house dust mite specificities in allergic disease. J Allergy Clin Immunol. 2006;118(2):361-7.
  43. Heymann PW, Chapman MD, Aalberse RC, Fox JW, Platts-Mills TA. Antigenic and structural analysis of group II allergens (Der f II and Der p II) from house dust mites (Dermatophagoides spp). J Allergy Clin Immunol. 1989;83(6):1055-67.
  44. Hong CS, Lee MK, Oh SH. Identification of major allergens from the house dust mites, Dermatophagoides farinae and Dermatophagoides pteronyssinus, by electroblotting. Yonsei Med J. 1991;32(1):24-32.
  45. Hong CS, Park JW, Nahm DH. Measurement of IgE and IgG subclass antibodies to whole body antigen and two major allergens (Der fI & Der fII) of

- Dermatophagoides farinae in normal subjects and asthmatics. *Yonsei Med J.* 1994;35(4):453-63.
46. Huang HW, Lue KH, Wong RH, Sun HL, Sheu JN, Lu KH. Distribution of allergens in children with different atopic disorders in central Taiwan. *Acta Paediatr Taiwan.* 2006;47(3):127-34.
  47. Jeong KY, Hwang H, Lee J, Lee IY, Kim DS, Hong CS, et al. Allergenic characterization of tropomyosin from the dusky brown cockroach, *Periplaneta fuliginosa*. *Clin Diagn Lab Immunol.* 2004;11(4):680-5.
  48. Jin HS, Yong TS, Park JW, Hong CS, Oh SH. Immune reactivity of recombinant group 2 allergens of house dust mite, *Dermatophagoides pteronyssinus*, and *Dermatophagoides farinae*. *J Investig Allergol Clin Immunol.* 2003;13(1):36-42.
  49. Jutel M, Akdis M, Budak F, Aebischer-Casaulta C, Wrzyszcz M, Blaser K, et al. IL-10 and TGF-beta cooperate in the regulatory T cell response to mucosal allergens in normal immunity and specific immunotherapy. *Eur J Immunol.* 2003 May;33(5):1205-14.
  50. Katoh N, Hirano S, Suehiro M, Masuda K, Kishimoto S. The characteristics of patients with atopic dermatitis demonstrating a positive reaction in a scratch test after 48 hours against house dust mite antigen. *J Dermatol.* 2004;31(9):720-6.
  51. Kawamoto S, Aki T, Yamashita M, Tategaki A, Fujimura T, Tsuboi S, et al. Toward elucidating the full spectrum of mite allergens state of the art. *J Biosci Bioeng.* 2002;94(4):285-98.
  52. Kawamoto S, Suzuki T, Aki T, Katsutani T, Tsuboi S, Shigeta S, et al. Der f 16: a novel gelsolin-related molecule identified as an allergen from the house dust mite, *Dermatophagoides farinae*. *FEBS Lett.* 2002;516(1-3):234-8.
  53. Khirwadkar K, Schmitz M, Kabelitz D. Frequency analysis of allergen-reactive T-lymphocytes in individuals allergic against the house-dust mite *Dermatophagoides pteronyssinus*. *Int Arch Allergy Immunol.* 1992;98(1):6-12.

54. Khosravi MJ, Diamandis EP. Immunofluorometry of choriogonadotropin by time-resolved fluorescence spectroscopy, with a new europium chelate as label. *Clin Chem*. 1987;33(11):1994-9.
55. Kidon MI, Chiang WC, Liew WK, Lim SH, See Y, Goh A, et al. Sensitization to dust mites in children with allergic rhinitis in Singapore: does it matter if you scratch while you sneeze? *Clin Exp Allergy*. 2005;35(4):434-40.
56. Kimura JY, Ohta N, Ishii A, Nagano T, Usui M. Functional characterization of lymphocyte response to fractionated house dust mite antigens (*Dermatophagoides pteronyssinus*) in atopic and non-atopic individuals. *Immunology*. 1990;70(3):385-90.
57. Kongpanichkul A, Vichyanond P, Tuchinda M. Allergen skin test reactivities among asthmatic Thai children. *J Med Assoc Thai*. 1997;80(2):69-75.
58. Koyanagi S, Maeda T, Murakami T, Kawatsu K, Sugawara K, Miyatsu Y, et al. Large-Scale Production of Major House Dust Mite Allergen Der f 2 Mutant (C8/119S) in *Escherichia coli*. *Journal of Bioscience and Bioengineering*. 2008;106(4):387-92.
59. Kramer U, Lemmen C, Bartusel E, Link E, Ring J, Behrendt H. Current eczema in children is related to Der f 1 exposure but not to Der p 1 exposure. *Br J Dermatol*. 2006;154(1):99-105.
60. Kuljanac I. The role of *Dermatophagoides pteronyssinus* in atopic dermatitis. *Acta Dermatovenerol Croat*. 2006;14(2):86-9.
61. Lai CL, Shyur SD, Wu CY, Chang CL, Chu SH. Specific IgE to 5 different major house dust mites among asthmatic children. *Acta Paediatr Taiwan*. 2002;43(5):265-70.
62. Lee AJ, Machell J, Van Den Broek AH, Nisbet AJ, Miller HR, Isaac RE, et al. Identification of an antigen from the sheep scab mite, *Psoroptes ovis*, homologous with house dust mite group I allergens. *Parasite Immunol*. 2002;24(8):413-22.
63. Lee CS, Tsai LC, Chao PL, Lin CY, Hung MW, Chien AI, et al. Protein sequence analysis of a novel 103-kDa *Dermatophagoides pteronyssinus* mite allergen and prevalence of serum immunoglobulin E reactivity to rDer p 11 in allergic adult patients. *Clin Exp Allergy*. 2004;34(3):354-62.

64. Leonard C, Tormey V, Burke C, Poulter LW. Allergen-induced cytokine production in atopic disease and its relationship to disease severity. *Am J Respir Cell Mol Biol.* 1997;17(3):368-75.
65. Lynch NR, Puccio FA, Di Prisco MC, Lopez RI, Hazell LA, Smith WA, et al. Reactivity to recombinant house-dust-mite allergens in asthma and rhinitis in a tropical environment. *Allergy.* 1998;53(8):808-11.
66. McGiven JA, Thompson IJ, Commander NJ, Stack JA. Time-resolved fluorescent resonance energy transfer assay for simple and rapid detection of anti-Brucella antibodies in ruminant serum samples. *J Clin Microbiol.* 2009;47(10):3098-107.
67. Meillet D, Belec L, Schuller E, Delattre J. Time-resolved fluoroimmunoassay of beta 2-microglobulin in serum and cerebrospinal fluid. *Clin Chem.* 1993;39(3):552-3.
68. Miyamoto T, Akiyama K, Ohta K, Urata C, Horiuchi Y. Studies in atopic asthma with emphasis on correlation among various tests and various antibodies. *J Allergy Clin Immunol.* 1981;67(4):279-84.
69. Noguchi E, Shibasaki M, Isoyama S, Takita H. Comparisons of IgE, IgG, and IgG4 responsiveness to *Dermatophagoides farinae* in children by immunoblotting. *Allergy.* 1996;51(12):907-13.
70. Noguchi E, Shibasaki M, Nishiyama C, Okumura Y, Takita H. IgE responsiveness to *Dermatophagoides farinae* in young asthmatic children: IgE binding study using recombinant allergens of Der f1, Der f2 and mutant proteins of Der f2. *Int Arch Allergy Immunol.* 1996;110(4):380-7.
71. Noguchi M, Yoshioka K, Kaneko H, Iwamura S, Takahashi T, Suzuki C, et al. Measurement of porcine luteinizing hormone concentration in blood by time-resolved fluoroimmunoassay. *J Vet Med Sci.* 2007;69(12):1291-4.
72. Nurse B, Puterman AS, Haus M, Berman D, Weinberg EG, Potter PC. PBMCs from both atopic asthmatic and nonatopic children show a TH2 cytokine response to house dust mite allergen. *J Allergy Clin Immunol.* 2000;106(1 Pt 1):84-91.

73. O'Brien RM, Thomas WR. Immune reactivity to Derp I and Der p II in house dust mite sensitive patients attending paediatric and adult allergy clinics. *Clin Exp Allergy*. 1994;24(8):737-42.
74. O'Hehir RE, Bal V, Quint D, Moqbel R, Kay AB, Zanders ED, et al. An in vitro model of allergen-dependent IgE synthesis by human B lymphocytes: comparison of the response of an atopic and a non-atopic individual to *Dermatophagoides* spp. (house dust mite). *Immunology*. 1989;66(4):499-504.
75. O'Neil SE, Heinrich TK, Hales BJ, Hazell LA, Holt DC, Fischer K, et al. The chitinase allergens Der p 15 and Der p 18 from *Dermatophagoides pteronyssinus*. *Clin Exp Allergy*. 2006;36(6):831-9.
76. Parra MD, Tuomola M, Cabezas-Herrera J, Ceron JJ. Analytical and clinical validation of a time-resolved immunofluorometric assay (TR-IFMA) for canine C-reactive protein in serum. *Vet Res Commun*. 2006;30(2):113-26.
77. Phipatanakul W, Cronin B, Wood RA, Eggleston PA, Shih MC, Song L, et al. Effect of environmental intervention on mouse allergen levels in homes of inner-city Boston children with asthma. *Ann Allergy Asthma Immunol*. 2004;92(4):420-5.
78. Pittner G, Vrtala S, Thomas WR, Weghofer M, Kundi M, Horak F, et al. Component-resolved diagnosis of house-dust mite allergy with purified natural and recombinant mite allergens. *Clin Exp Allergy*. 2004;34(4):597-603.
79. Platts-Mills TA, Chapman MD. Dust mites: immunology, allergic disease, and environmental control. *J Allergy Clin Immunol*. 1987;80(6):755-75.
80. Pumhirun P, Towiwat P, Mahakit P. Aeroallergen sensitivity of Thai patients with allergic rhinitis. *Asian Pac J Allergy Immunol*. 1997;15(4):183-5.
81. Richards D, Chapman MD, Sasama J, Lee TH, Kemeny DM. Immune memory in CD4+ CD45RA+ T cells. *Immunology*. 1997;91(3):331-9.
82. Sanchez-Borges M, Capriles-Hulett A, Fernandez-Caldas E, Suarez-Chacon R, Caballero F, Castillo S, et al. Mite-contaminated foods as a cause of anaphylaxis. *J Allergy Clin Immunol*. 1997;99(6 Pt 1):738-43.

83. Santos AB, Chapman MD, Aalberse RC, Vailes LD, Ferriani VP, Oliver C, et al. Cockroach allergens and asthma in Brazil: identification of tropomyosin as a major allergen with potential cross-reactivity with mite and shrimp allergens. *J Allergy Clin Immunol.* 1999;104(2 Pt 1):329-37.
84. Satinover SM, Reefer AJ, Pomes A, Chapman MD, Platts-Mills TA, Woodfolk JA. Specific IgE and IgG antibody-binding patterns to recombinant cockroach allergens. *J Allergy Clin Immunol.* 2005;115(4):803-9.
85. Sato T, Kajikuri T, Saito Y, Chikuma M, Nagai S. Determination of desmosine in bronchoalveolar lavage fluids by time-resolved fluoroimmunoassay. *Clin Chim Acta.* 2008;387(1-2):113-9.
86. Sell SB, Max EE. *Immunology, Immunopathology, and Immunity.* 6<sup>th</sup> ed. Washington DC. 2001.
87. Sewell WAC, Dore PC. Premature testing of allergen-specific IgE post-anaphylaxis may cause false negative results. *J Allergy Clin Immunol.* 2004;113:S241.
88. Shen HD, Chua KY, Lin WL, Hsieh KH, Thomas WR. Molecular cloning and immunological characterization of the house dust mite allergen Der f 7. *Clin Exp Allergy.* 1995;25(10):1000-6.
89. Shen HD, Lin WL, Tsai LC, Tam MF, Chua KY, Chen HL, et al. Characterization of the allergen Der f 7 from house dust mite extracts by species-specific and crossreactive monoclonal antibodies. *Clin Exp Allergy.* 1997;27(7):824-32.
90. Sheng SL, Bao SH, Huang G, Wang LM. Development of time-resolved immunofluorometric assays for vascular endothelial growth factor and application on plasma of patients with gastric tumours. *Clin Exp Immunol.* 2008;151(3):459-66.
91. Slunt JB, Taketomi EA, Platts-Mills TA. Human T-cell responses to *Trichophyton tonsurans*: inhibition using the serum free medium Aim V. *Clin Exp Allergy.* 1997;27(10):1184-92.
92. Sidenius KE, Hallas TE, Poulsen LK, Mosbech H. Allergen cross-reactivity between house-dust mites and other invertebrates. *Allergy.* 2001;56(8):723-33.



93. Sidenius KE, Hallas TE, Poulsen LK, Mosbech H. House dust mites and their allergens in Danish mattresses results from a population based study. *Ann Agric Environ Med.* 2002;9(1):33-9.
94. Siitari H, Hemmilä I, Soini E, Lövgren T, Koistinen V. Detection of hepatitis B surface antigen using time-resolved fluoroimmunoassay. *Nature.* 1983;301:258-60.
95. Smith AM, Yamaguchi H, Platts-Mills TA, Fu SM. Prevalence of IgG anti-Der p 2 antibodies in children from high and low antigen exposure groups: relationship of IgG and subclass antibody responses to exposure and allergic symptoms. *Clin Immunol Immunopathol.* 1998;86(1):102-9.
96. Smith WA, Chua KY, Kuo MC, Rogers BL, Thomas WR. Cloning and sequencing of the *Dermatophagoides pteronyssinus* group III allergen, Der p III. *Clin Exp Allergy.* 1994;24(3):220-8.
97. Soares FA, Segundo GR, Alves R, Ynoue LH, Resende RO, Sopelete MC, et al. [Indoor allergen sensitization profile in allergic patients of the allergy clinic in the University Hospital in Uberlandia, Brazil]. *Rev Assoc Med Bras.* 2007;53(1):25-8.
98. Soini E, Kojola H. Time-resolved fluorometer for lanthanide chelates-a new generation of nonisotopic immunoassays. *Clin Chem.* 1983;29(1):65-8.
99. Solarz K, Senczuk L, Maniurka H, Cichecka E, Peszke M. Comparisons of the allergenic mite prevalence in dwellings and certain outdoor environments of the Upper Silesia (southwest Poland). *Int J Hyg Environ Health.* 2007;210(6):715-24.
100. Spieksma FT. Biological aspects of the house dust mite (*Dermatophagoides pteronyssinus*) in relation to house dust atopy. *Clin Exp Immunol.* 1970;6(1):61-70.
101. Sporik R, Holgate ST, Platts-Mills TA, Cogswell JJ. Exposure to house-dust mite allergen (Der p I) and the development of asthma in childhood. A prospective study. *N Engl J Med.* 1990;323(8):502-7.
102. Sporik R, Ingram JM, Price W, Sussman JH, Honsinger RW, Platts-Mills TA. Association of asthma with serum IgE and skin test reactivity to allergens

- among children living at high altitude. Tickling the dragon's breath. *Am J Respir Crit Care Med*. 1995;151(5):1388-92.
103. Stewart GA, Kollinger MR, King CM, Thompson PJ. A comparative study of three serine proteases from *Dermatophagoides pteronyssinus* and *D. farinae*. *Allergy*. 1994;49(7):553-60.
  104. Sun JL, Wang RQ, Yin J, Wang LL, Zhang HY, Li H, et al. Comparison and evaluation of several *Dermatophagoides pteronyssinus* allergen extracts for skin prick test. *Med Sci J*. 2009;24(2):86-90.
  105. Suzuki M, Tanaka Y, Korematsu S, Mikami B, Minato N. Crystal structure and some properties of a major house dust mite allergen, Derf 2. *Biochemical and Biophysical Research Communications*. 2006;339:679-86.
  106. Takai T, Kato T, Yasueda H, Okumura K, Ogawa H. Analysis of the structure and allergenicity of recombinant pro- and mature Der p 1 and Der f 1: major conformational IgE epitopes blocked by prodomains. *J Allergy Clin Immunol*. 2005;115(3):555-63.
  107. Tategaki A, Kawamoto S, Aki T, Jyo T, Suzuki O, Shigeta S, et al. Newly described house dust mite allergens. *ACI International suppl*. 2000;1:74-6.
  108. Taylor G, Walker J. Charles Harrison Blackley, 1820-1900. *Clin Allergy*. 1973;3:103-8.
  109. Teeratakulpisarn J, Pairojkul S, Heng S. Survey of the prevalence of asthma, allergic rhinitis and eczema in schoolchildren from Khon Kaen, Northeast Thailand. an ISAAC study. *International Study of Asthma and Allergies in Childhood*. *Asian Pac J Allergy Immunol*. 2000;18(4):187-94.
  110. Thomas WR, Smith W. House-dust-mite allergens. *Allergy*. 1998;53(9):821-32.
  111. Thomas WR, Smith WA, Hales BJ. The allergenic specificities of the house dust mite. *Chang Gung Med J*. 2004;27(8):563-9.
  112. Tsai JJ, Chen WC. Different age of asthmatic patients affected by different aeroallergens. *J Microbiol Immunol Infect*. 1999;32(4):283-8.

113. Tsai L, Sun Y, Chao P, Ng H, Hung M, Hsieh K, et al. Sequence analysis and expression of a cDNA clone encoding a 98-kDa allergen in *Dermatophagoides farinae*. *Clin Exp Allergy*. 1999;29(12):1606-13.
114. Tsai LC, Chao PL, Hung MW, Sun YC, Kuo IC, Chua KY, et al. Protein sequence analysis and mapping of IgE and IgG epitopes of an allergenic 98-kDa *Dermatophagoides farinae* paramyosin, Der f 11. *Allergy*. 2000;55(2):141-7.
115. Tsai LC, Chao PL, Shen HD, Tang RB, Chang TC, Chang ZN, et al. Isolation and characterization of a novel 98-kd *Dermatophagoides farinae* mite allergen. *J Allergy Clin Immunol*. 1998;102(2):295-303.
116. Tsai LC, Peng HJ, Lee CS, Chao PL, Tang RB, Tsai JJ, et al. Molecular cloning and characterization of full-length cDNAs encoding a novel highmolecular-weight *Dermatophagoides pteronyssinus* mite allergen, Der p 11. *Allergy*. 2005;60(7):927-37.
117. Van Der Veen MJ, Jansen HM, Aalberse RC, van der Zee JS. Der p 1 and Der p 2 induce less severe late asthmatic responses than native *Dermatophagoides pteronyssinus* extract after a similar early asthmatic response. *Clin Exp Allergy*. 2001;31(5):705-14.
118. Vichyanond P. HDM, the major allergens sensitized asthmatic Thai children. *Siriraj hospital Gaz*. 1998;48:719-21.
119. Warner A, Bostrom S, Munir AK, Moller C, Schou C, Kjellman NI. Environmental assessment of *Dermatophagoides* mite-allergen levels in Sweden should include Der m 1. *Allergy*. 1998;53(7):698-704.
120. Westritschnig K, Sibanda E, Thomas W, Auer H, Aspöck H, Pittner G, et al. Analysis of the sensitization profile towards allergens in central Africa. *Clin Exp Allergy*. 2003;33(1):22-7.
121. Wharton GW. House dust mites. *J Med Entomol*. 1976;12(6):577-621.
122. Williams P, Sewell WA, Bunn C, Pumphrey R, Read G, Jolles S. Clinical immunology review series: an approach to the use of the immunology laboratory in the diagnosis of clinical allergy. *Clin Exp Immunol*. 2008;153(1):10-8.

123. Wood RA, Eggleston PA, Lind P, Ingemann L, Schwartz B, Graveson S, et al. Antigenic analysis of household dust samples. *Am Rev Respir Dis.* 1988;137(2):358-63.
124. Wu FB, Ouyan HQ, Tang XY, Zhou ZX. Double-antigen sandwich time-resolved immunofluorometric assay for the detection of anti-hepatitis C virus total antibodies with improved specificity and sensitivity. *J Med Microbiol.* 2008;57(Pt 8):947-53.
125. Yang QG, Li CP. Cloning, sequencing and subcloning of cDNA coding for group I allergen of *Dermatophagoides farinae*. *Zhongguo Ji Sheng Chong Xue Yu Ji Sheng Chong Bing Za Zhi.* 2004;22(3):173-5.
126. Yasueda H, Mita H, Akiyama K, Shida T, Ando T, Sugiyama S, et al. Allergens from *Dermatophagoides* mites with chymotryptic activity. *Clin Exp Allergy.* 1993;23(5):384-90.
127. Yasueda H, Mita H, Yui Y, Shida T. Comparative analysis of physicochemical and immunochemical properties of the two major allergens from *Dermatophagoides pteronyssinus* and the corresponding allergens from *Dermatophagoides farinae*. *Int Arch Allergy Appl Immunol.* 1989;88(4):402-7.
128. Yasuhara T, Takai T, Yuuki T, Okudaira H, Okumura Y. Cloning and expression of cDNA encoding the complete preproform of an isoform of Der f 1, the major group 1 allergen from house dust mite *Dermatophagoides farinae*. *Biosci Biotechnol Biochem.* 2001;65(3):563-9.
129. Yi FC, Cheong N, Shek PC, Wang DY, Chua KY, Lee BW. Identification of shared and unique immunoglobulin E epitopes of the highly conserved tropomyosins in *Blomia tropicalis* and *Dermatophagoides pteronyssinus*. *Clin Exp Allergy.* 2002;32(8):1203-10.
130. Young RP, Hart BJ, Faux JA, Hopkin JM. House dust mite sensitivity: a comparison of immune response with exposure to four species of *Pyroglyphidae*. *Clin Exp Allergy.* 1990;20(3):319-25.
131. Yuan AS, Gilbert JD. Time-resolved fluoroimmunoassay for the determination of lisinopril and enalaprilat in human serum. *J Pharm Biomed Anal.* 1996;14(7):773-81.

132. Zhu YF, Liu ZG, Gao B. Cloning, expression, purification and identification of Der f6 gene and its immunological characteristics from the dust house mite. *Zhongguo Ji Sheng Chong Xue Yu Ji Sheng Chong Bing Za Zhi.* 2006;24(4):241-6.
133. Zock JP, Heinrich J, Jarvis D, Verlato G, Norback D, Plana E, et al. Distribution and determinants of house dust mite allergens in Europe: the European Community Respiratory Health Survey II. *J Allergy Clin Immunol.* 2006;118(3):682-90.

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

APPENDIX  
มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

**APPENDIX A**

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

### List of Abbreviations

Abbreviation	Term
A	Allergic
APCs	Antigen presenting cells
BMGY	buffered minimal glycerol complex medium
BMMY	buffered minimal methanol complex medium
Bt	<i>Blomia tropicalis</i>
BSA	bovine serum albumine
CR	American Cockroach
°C	degree Celsius
cm	centimeter
cts	counts per second
DAS-TR-IFMA	Double-antigen Sandwich Time-resolved immunofluorometric assay
Der	<i>Dermatophagoides</i>
Df	<i>Dermatophagoides farinae</i>
Dp	<i>Dermatophagoides pteronyssinus</i> ;
ELISA	Enzyme Link Immuno Sorbent Assay
EU	europium
et al	et alia
F	Female
FPA	Fluorescence polarization assay
H	Healthy
HDM	House Dust Mite
h	hour (s)
IL	interleukin
IFN	interferon
IUIS	International Union of Immunological Societies
Ig	Immunoglobulin
kDa	kilo Dalton
kU <sub>A</sub> /l	kilo units of aprotinin-specific antibodies per liter



Abbreviation	Term
M	Male
mAb	monoclonal antibody
mg	milligram
min	minute (s)
ml	milliliter
mm	millimeter
μg	microgram
μl	microliter
nm	nanometer
OD	optical density
<i>P. pastoris</i>	<i>Pichia pastoris</i>
PBS	phosphate buffer saline
rpm	round per minute
SDS-PAGE	Sodium Dodecyl Sulfate Polyacrylamide gel Electrophoresis
SPT	Skin prick Test
SMM	Spent Mite Medium
TRF	Time-resolved Fluoroimmunoassay
TR-FRET	Time-resolved Fluorescent resonance energy transfer
TR-IFMA	Time-resolved Immunofluorometric assay
V	volt
VEGF	vascular endothelial growth factor
v/v	volume / volume
w/v	weight / volume
YPD	yeast extract peptone dextrose

**APPENDIX B**

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์

## General Reagents

### Phosphate Buffered Saline (PBS), pH 7.4

NaCl	8.0	g
KH <sub>2</sub> PO <sub>4</sub>	0.24	g
Na <sub>2</sub> HPO <sub>4</sub>	1.44	g
KCl	0.20	g

Dissolve in deionized water, adjust to pH 7.4 with HCl and adjust to final volume of 1,000 ml with deionized water. Sterized by autoclave.

## Culture Media

### Yeast Extract Peptone (YP)

yeast extract	1.0	g
tryptone	2.0	g

Dissolve and adjust the volume of 90 ml with deionized water. Sterized by autoclave at 121 °C, 15 lb/square inches for 15 min.

### 10X Dextrose (D)

Dextrose	5.0	g
----------	-----	---

Dissolve and adjust the volume of 25 ml with deionized water. Sterized by autoclave.

### Buffered minimal (BM)

yeast extract	5.0	g
tryptone	10.0	g

Dissolve and adjust the volume of 350 ml with deionized water. Sterized by autoclave.

### 1 M K<sub>2</sub>HPO<sub>4</sub>

K <sub>2</sub> HPO <sub>4</sub>	8.709	g
---------------------------------	-------	---

Dissolve and adjust the volume of 50 ml with deionized water.

### 1M KH<sub>2</sub>PO<sub>4</sub>

KH <sub>2</sub> PO <sub>4</sub>	13.609	g
---------------------------------	--------	---

Dissolve and adjust the volume of 100 ml with deionized water.

### 1M Potassium Phosphate Buffer, pH 6.0

1 M K <sub>2</sub> HPO <sub>4</sub>	13.2	ml
-------------------------------------	------	----

1M KH <sub>2</sub> PO <sub>4</sub>	86.8	ml
------------------------------------	------	----

Dissolve in deionized water, adjust to pH 6.0 and sterilized by autoclave at 121 °C, 15 lb/square inches for 15 minutes.

**10X 13.4% Yeast Nitrogen Base with (NH<sub>4</sub>)<sub>2</sub>SO<sub>4</sub> but without amino acid (YNB)**

YNB	13.4	ml
-----	------	----

Dissolve and adjust the volume of 100 ml with deionized water. Sterilized by 0.22 μ filter and store at night.

**10X Glycerol**

Glycerol	5.0	ml
----------	-----	----

Dissolve and adjust the volume of 45 ml with deionized water. Sterilized by autoclave.

**10X Methanol**

Methanol	3.0	ml
----------	-----	----

Dissolve and adjust the volume of 97 ml with deionized water. Sterilized by autoclave.

**500X Biotin**

Biotin	2.0	g
--------	-----	---

Dissolve and adjust the volume of 10 ml with deionized water. Sterilized by 0.22 μ filter and store at night.

**Yeast extract peptone dextrose (YPD)**

YP	9.0	ml
----	-----	----

10X D	1.0	ml
-------	-----	----

Zeocin <sup>TM</sup> (100 μg/ml)	10.0	μl
----------------------------------	------	----

**Buffered minimal glycerol complex medium (BMGY)**

BM	70.0	ml
----	------	----

1M Potassium Phosphate Buffer	10.0	ml
-------------------------------	------	----

10X YNB	10.0	ml
---------	------	----

10X GY	10.0	ml
--------	------	----

500X B	100.0	μl
--------	-------	----

**Buffered minimal methanol complex medium (BMMY)**

BM	70.0	ml
----	------	----

1M Potassium Phosphate Buffer	10.0	ml
10X YNB	10.0	ml
10X M	10.0	ml
500X B	100.0	μl

### Reagent for Polyacrylamine Gel Electrophoresis

#### Lower gel buffer

Tris base	18.2	g
Sodium dodecyl sulfate (SDS)	0.4	g

Dissolve in deionized water, adjust to pH 8.8 and adjust to final volume of 100 ml with deionized water.

#### Upper gel buffer

Tris base	6.0	g
SDS	0.4	g

Dissolve in deionized water, adjust to pH 6.8 and adjust to final volume of 100 ml with deionized water.

#### 10% Ammonium persulfate (APS) (w/v)

Ammonium persulfate	1.0	g
Deionized water	10.0	ml

#### 12.5% Resolving gel

Lower gel buffer	1.0	ml
Deionized water	1.33	ml
30% Acrylamide	1.67	ml
10% APS	20.0	μl
TEMED	8.0	μl

#### 4% Resolving gel

Upper gel buffer	0.78	ml
Deionized water	1.83	ml
30% Acrylamind	0.39	ml
10% APS	20.0	μl
TEMED	5.0	μl

#### 4X Sample buffer

Glycerol	4.0	ml
SDS	0.4	g
Upper gel buffer	5.0	ml
Bromophenol blue	2.0	g
2- Mercaptoethanol	1.0	ml

Dissolve and adjust the volume of 10 ml with deionized water.

#### **10X Electrode buffer**

Tris base	30.0	g
Glycine	144.0	g
SDS	10.0	g

Dissolve in deionized water, adjust to pH 8.3 and adjust to final volume of 1,000 ml with deionized water.

#### **Working Electrode buffer**

10X Electrode buffer	100	ml
----------------------	-----	----

Dissolve and adjust the volume of 900 ml with deionized water.

#### **Coomassie Brilliant Blue (CBB)**

CBB-G 250 stock	5	g]
Ammonium sulfate	50	g
85% O-phosphoric acid (w/w)	6	ml
Methanol	125	ml

Dissolve and adjust to final volume of 500 ml with deionized water.

#### **5% SDS**

SDS	0.25	g
-----	------	---

Dissolve and adjust to final volume of 5 ml with deionized water.

#### **7.5X Electroblotting buffer**

Tris base	4.5375	g
Glycine	21.6	g

Dissolve and adjust to final volume of 200 ml with deionized water.

#### **Working Electroblotting buffer**

7.5X Electroblotting buffer	200	ml
Methanol	300	ml
5% SDS	3	ml

Dissolve and adjust to final volume of 1500 ml with deionized water.

**0.1 % PBS-Tween 20 (PBS-T)**

PBS	1,000	ml
Tween 20	1	ml

**Blocking/Diluting buffer (PBST with 3% BSA)**

PBS-T	100	ml
BSA	3	g

**Reagent for Enzyme-Linked Immunosorbent assay**

**50mM carbonate/bicarbonate buffer, pH 9.6**

Na <sub>2</sub> CO <sub>3</sub>	1.59	g
NaHCO <sub>3</sub>	2.93	g

Dissolve in deionized water, adjust pH to 9.6 and adjust to 1,000 ml final volume with deionized water. Sterized by autoclave.

**0.05% PBS-Tween (PBS-T)**

PBS	1,000	ml
Tween 20	0.5	ml

**Blocking/Diluting buffer (PBST with 1% BSA)**

PBS-T	100	ml
BSA	1	g

**APPENDIX C**

มหาวิทยาลัยศิลปากร สงวนลิขสิทธิ์



**ข้อมูลสำหรับผู้เข้าร่วมโครงการวิจัย**  
**(Patient/Participant Information Sheet)**

**ชื่อโครงการ** การตรวจวัดระดับ IgE ต่อสารก่อภูมิแพ้จากไรฝุ่นด้วย time-resolved fluoroimmunoassay

การตรวจวินิจฉัยหาสาเหตุของการเกิดโรคภูมิแพ้ของผู้ป่วยสามารถทำได้หลายวิธี เช่น การทดสอบภูมิแพ้ทางผิวหนังของผู้ป่วยโดยตรงด้วยวิธี skin test พบว่ามีความไวสูงแต่ไม่จำเพาะเจาะจงขณะที่การตรวจวัดระดับ IgE ด้วยวิธี ELISA test มีความไวต่ำกว่าวิธีแรกแต่มีความจำเพาะเจาะจงมากกว่า จากรายงานของต่างประเทศพบว่า time-resolved fluoroimmunoassay มีความไวและความจำเพาะเจาะจงสูง ด้วยเหตุนี้ผู้วิจัยจึงต้องการที่จะพัฒนาเทคนิคนี้ขึ้นในประเทศไทย เพื่อเป็นประโยชน์ต่อผู้ป่วยในการวินิจฉัยโรคภูมิแพ้ต่อไป

วิธีดำเนินการแพทย์ผู้ดูแลรักษาจะทำการซักประวัติ ตรวจร่างกาย วัดความดันโลหิตชีพจร และเก็บตัวอย่างเลือดจากผู้ป่วยโดยการเจาะเส้นเลือดดำบริเวณข้อพับแขนปริมาณ 10 มิลลิลิตร ตามวิธีมาตรฐานการดำเนินการเจาะเลือด

เด็กในปกครองของท่านหรือตัวท่านเองจะได้รับการดูแลในโรงพยาบาลเป็นเวลาประมาณ 30 นาที หลังได้รับการเจาะเลือด โดยไม่เสียค่าใช้จ่าย และพิจารณาให้กลับบ้านได้หากไม่พบอาการผิดปกติ

ในระหว่างการดำเนินการเจาะเลือด เด็กหรือตัวท่านเองจะได้รับการดูแลอย่างใกล้ชิด กรณีที่ท่านมีข้อสงสัยขอให้ท่านติดต่อสอบถามแพทย์ผู้ดำเนินการเจาะเลือดได้ทันที

การยินยอมเข้าร่วมโครงการนี้เป็นไปโดยความสมัครใจ ท่านสามารถปฏิเสธ หรือขอยกเลิกการเข้าร่วมโครงการได้ตลอดเวลา

ข้อมูลที่ได้จากโครงการนี้ จะถูกจัดเก็บไว้ในคอมพิวเตอร์อย่างน้อย 15 ปี และจะไม่มีการระบุชื่อผู้ที่เข้าร่วมโครงการ มีเพียงแพทย์เท่านั้นที่รู้ว่าข้อมูลใดเกี่ยวข้องกับเด็กในกรณีที่มีการตีพิมพ์ผลของการเจาะเลือดในวารสารทางการแพทย์และวารสารอื่น ๆ ในระดับนานาชาติ เพื่อเป็นการรักษาความลับจะไม่มีการเปิดเผยชื่อเด็กในปกครองของท่าน

ในกรณีที่ท่านมีข้อสงสัยเกี่ยวกับโครงการ กรุณาติดต่อ แพทย์หญิง นารศ วงศ์ไพฑูริย์ หรือ แพทย์หญิง วรวรรณ ศุภกิจพิศุภกุล ได้ที่ งานกุมารเวชกรรม โรงพยาบาลตำรวจ หมายเลขโทรศัพท์ 0-2517-4270-9 ต่อ 1459 หมายเลขโทรสาร 0-2652-5033 และ/หรือ อาจารย์ ดร. จันตรีดี ระเบียบเลิศ หมายเลขโทรศัพท์ 084-7102575 ภาควิชาชีววิทยา คณะวิทยาศาสตร์ มหาวิทยาลัยศิลปากร วิทยาเขตพระราชวังสนามจันทร์ จ.นครปฐม

ใบยินยอมเข้าร่วมโครงการวิจัย  
(Informed Consent Form)

ชื่อโครงการ การตรวจวัดระดับ IgE ต่อสารก่อภูมิแพ้จากไรฝุ่นด้วย time-resolved fluoroimmunoassay

ข้าพเจ้า.....(บิดา มารดา/ผู้ปกครอง)

ที่อยู่.....

หมายเลขโทรศัพท์.....ได้อ่านเอกสารรายละเอียดโครงการที่มีชื่อข้างต้น

และได้มีโอกาสซักถามเกี่ยวกับโครงการนี้จาก แพทย์หญิงนารศ วงศ์ไพฑูรย์ หรือ  
แพทย์หญิงวรรณ ศุรงค์พิศิษฐ์กุล และเข้าใจโครงการนี้

ข้าพเจ้ายินยอมให้.....(บุตร/ธิดา/ตนเอง)

อายุ.....ปี เลขที่โรงพยาบาล.....เข้าร่วมในโครงการ

หากข้าพเจ้ามีข้อสงสัยเกี่ยวกับการดำเนินการเจาะเลือด ข้าพเจ้ามีสิทธิซักถามแพทย์ได้ใน  
ระหว่างการดำเนินการเจาะเลือดและคำชี้แจงของแพทย์ผู้ดำเนินการเจาะเลือดยังไม่เป็นที่เข้าใจ

ข้าพเจ้ามีสิทธิแจ้งต่อประธานคณะกรรมการจริยธรรมการวิจัยในมนุษย์ หมายเลขโทรศัพท์

0-2252-8111-25 ต่อ 4135 หรือผู้บังคับการ โรงพยาบาลตำรวจ หมายเลขโทรศัพท์ 0-2252-8111-25

ต่อ 4222 ได้ และหากข้าพเจ้าไม่พอใจในการดำเนินการเจาะเลือด ข้าพเจ้ามีสิทธิปฏิเสธการ

ดำเนินการเจาะเลือดวิธีนี้ได้ทันที โดยไม่เสียสิทธิในการรักษาในโรงพยาบาลต่อไป

ข้าพเจ้าได้อ่านและเข้าใจเกี่ยวกับการดำเนินการเจาะเลือดทั้งหมดตามคำอธิบายข้างต้น

แล้ว ข้าพเจ้ายินยอมรับการดำเนินการเจาะเลือดตามวิธีดังกล่าว

.....

ลายเซ็นของบิดา มารดา/ผู้ปกครอง/ตนเอง

.....

วัน/เดือน/ปี

.....

ลายเซ็นของพยาน

.....

วัน/เดือน/ปี

.....

ลายเซ็นของพยาน

.....

วัน/เดือน/ปี

.....

ลายเซ็นของแพทย์

.....

วัน/เดือน/ปี

**BIOGRAPHY**

Name MissRatchanoo Phiphatchaipaisarn  
 Home Address 27, Soi Taksin 22, Taksin Road, Thonburi,  
 Bangkok, 10600  
 Office Address 55/18 Moo 2, Samkoh, Sena, Ayutthaya, 13110

**Education Background**

2004 Bachelor of Science, Department of pest  
 management technology, Faculty of Aricultural  
 Technology, King Mongkut's Institute of  
 Technology Ladkrabang

2010 Master of Science, Department of Biology, Faculty  
 of Science, Graduate School, Silpakorn University

**Working Experience**

2005-2007 Staff in the project house dust mite, Department of  
 Parasitology, Faculty of Medicine Siriraj Hospital,  
 Mahidol University

2010-present Business Development staff at Bank for  
 Agriculture and Agricultural Co-operatives

มหาวิทยาลัยศิลปากร สงวนลขลภกร